

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 04/17/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:29
INTERNAL STANDARD	VERIFIED	01:29
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:29
BLANK TEST	0.00	01:30
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	01:31
BLANK TEST	0.00	01:31
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	01:32
BLANK TEST	0.00	01:33

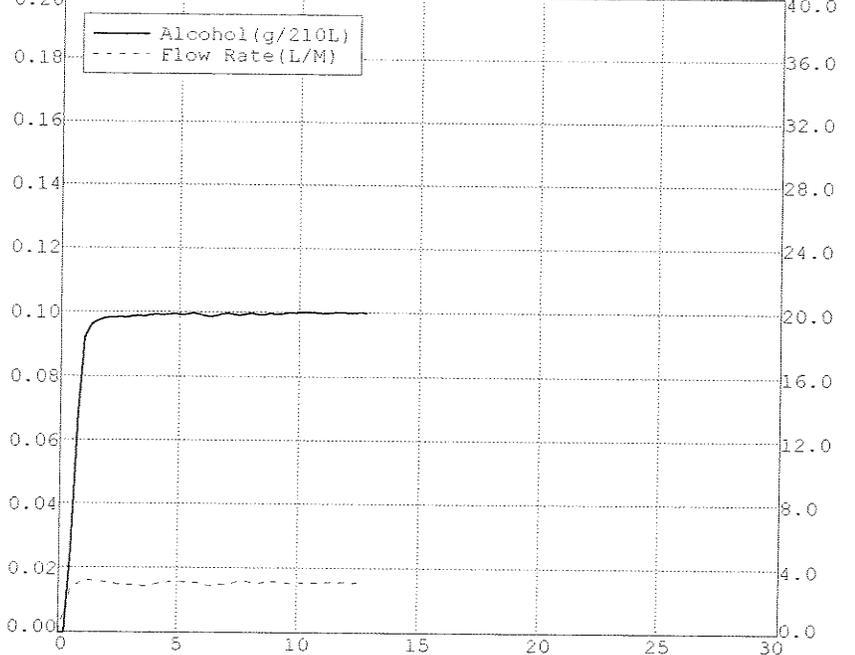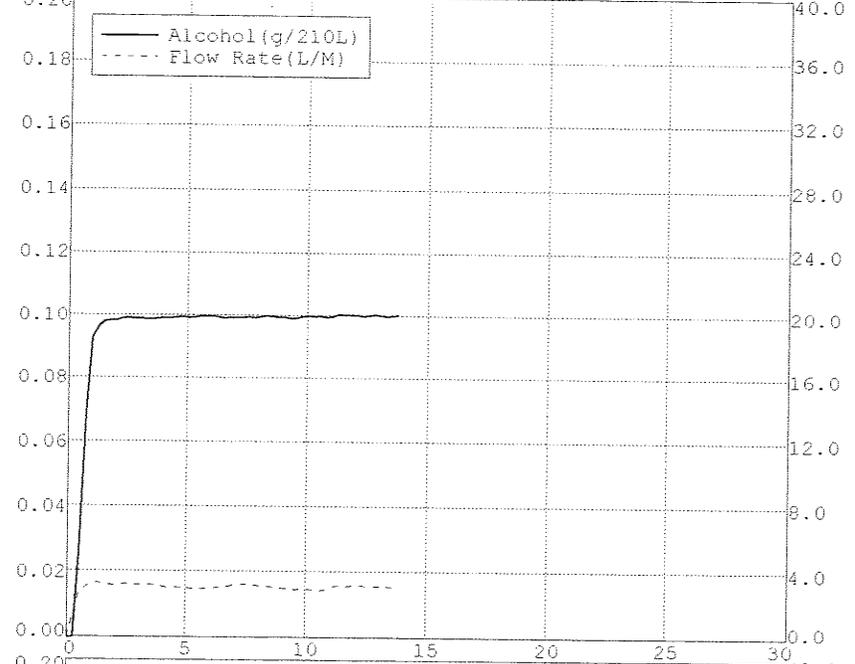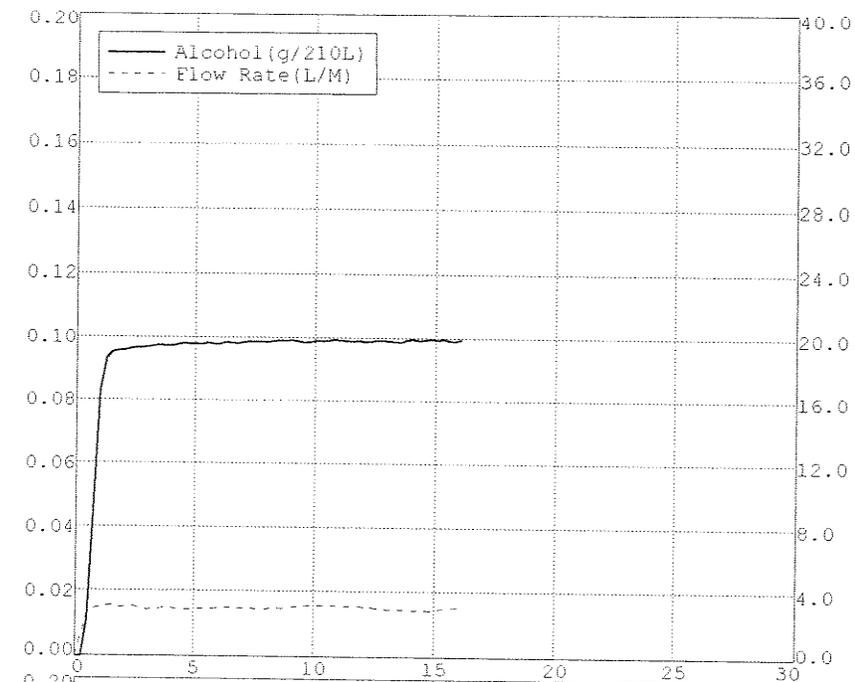

Charles B. Geisler #245