

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 04/24/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:51
INTERNAL STANDARD	VERIFIED	23:51
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	23:52
BLANK TEST	0.00	23:53
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	23:53
BLANK TEST	0.00	23:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:54
BLANK TEST	0.00	23:55

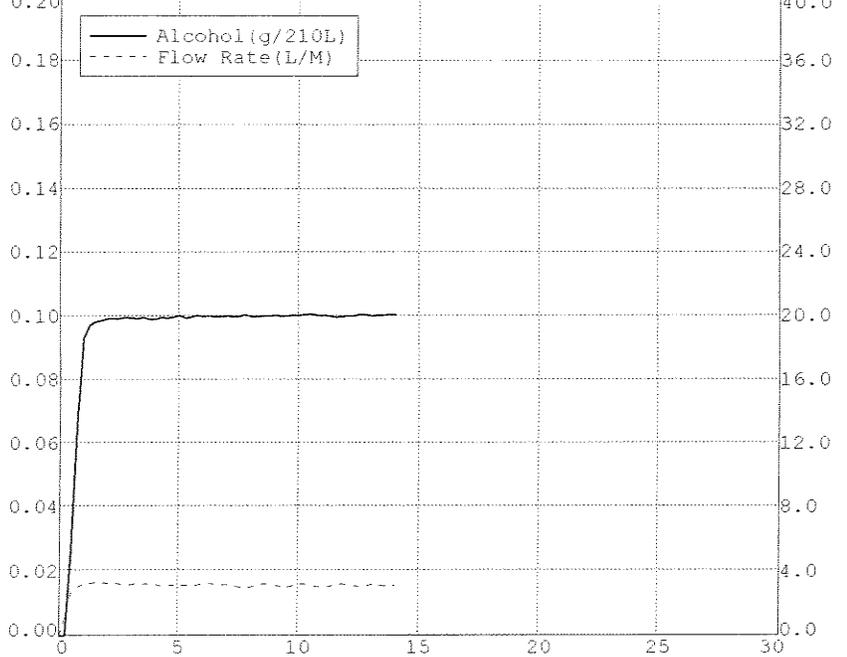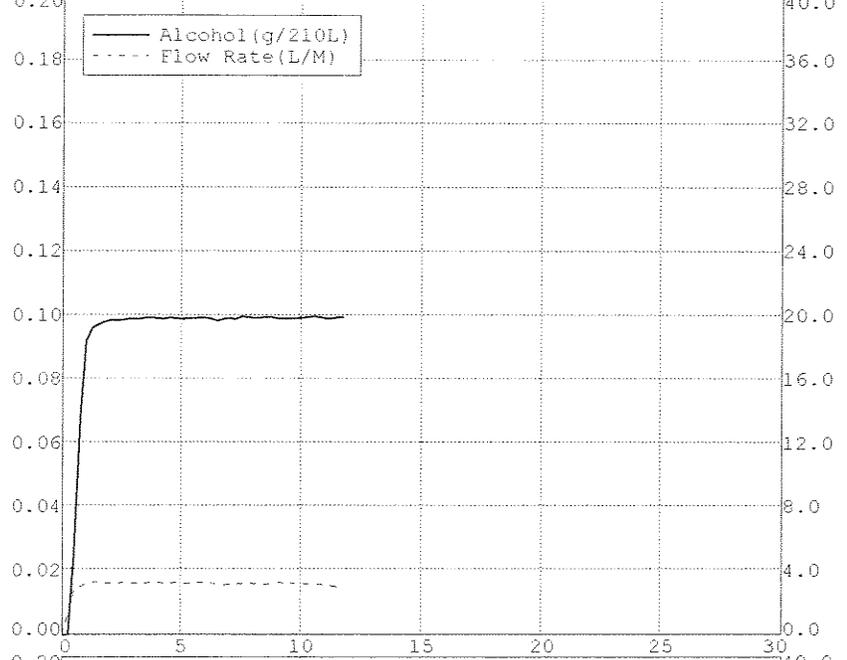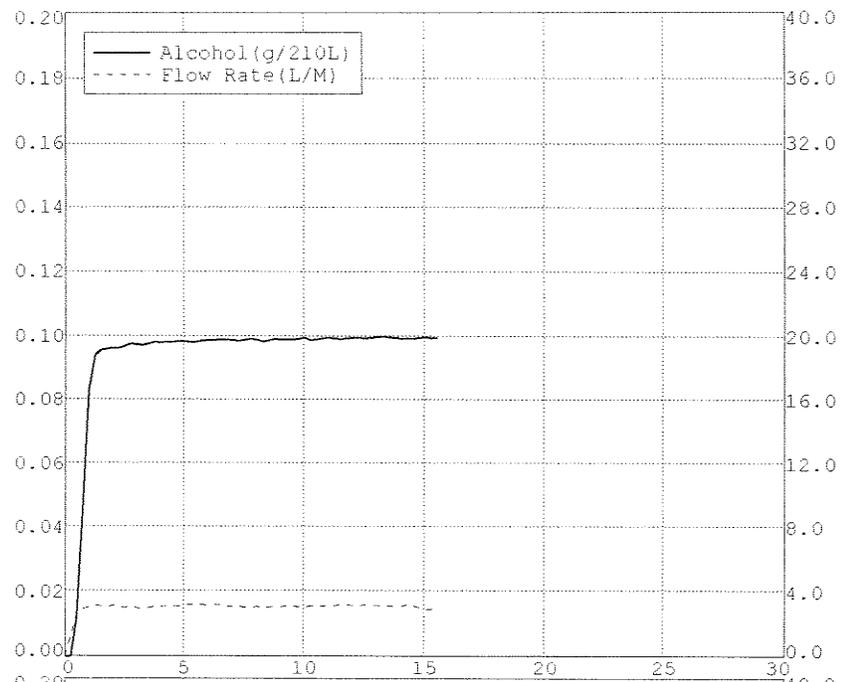

Charles B. Geisler #295