

SUPERVISOR TEST


WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 106606

Date: 05/08/2019

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:01
INTERNAL STANDARD	VERIFIED	19:01
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	19:01
BLANK TEST	0.00	19:02
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	19:03
BLANK TEST	0.00	19:04
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	19:04
BLANK TEST	0.00	19:05

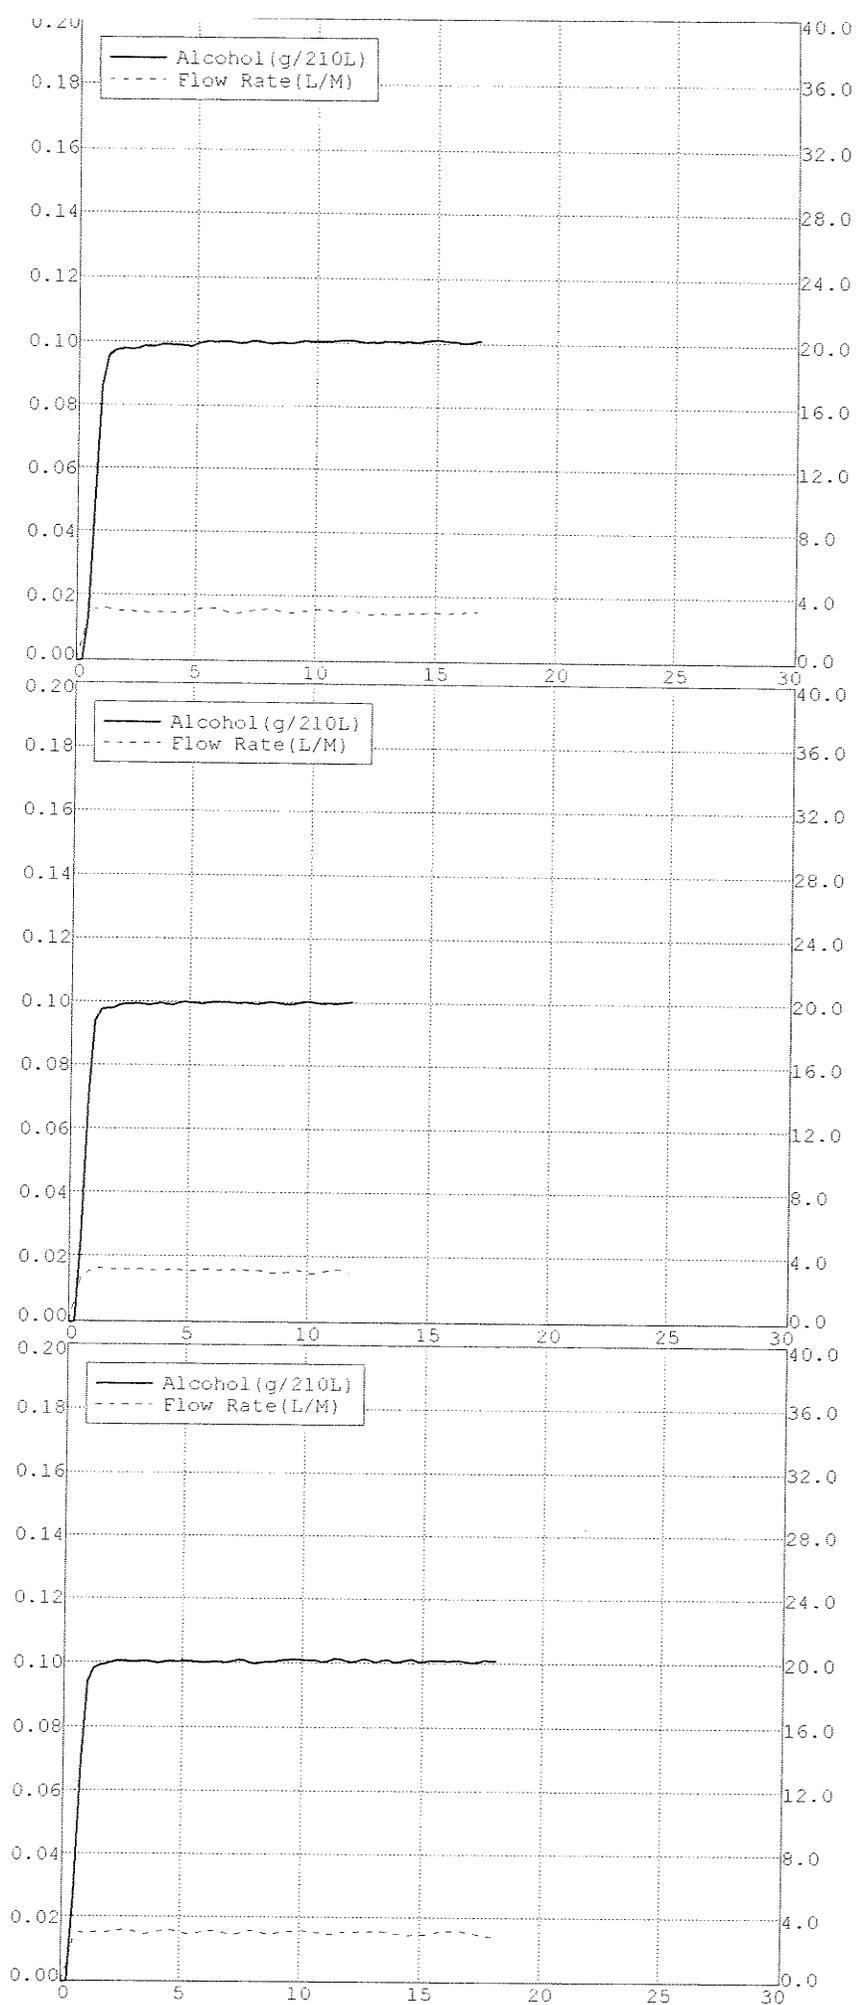

*Charles B. Geisler* #241