

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 05/15/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:57
INTERNAL STANDARD	VERIFIED	00:57
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	00:58
BLANK TEST	0.00	00:59
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	00:59
BLANK TEST	0.00	01:00
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	01:00
BLANK TEST	0.00	01:01

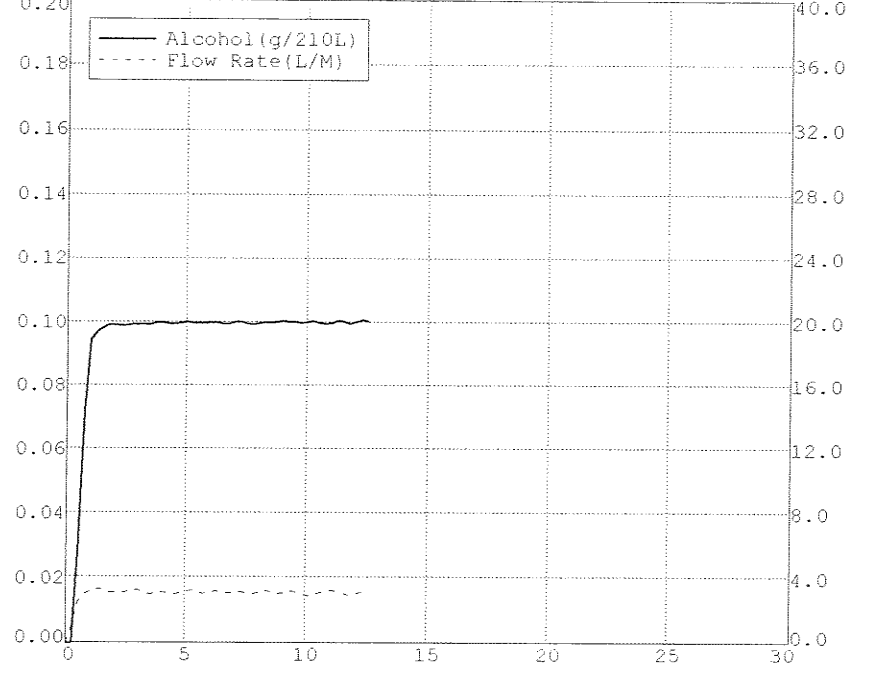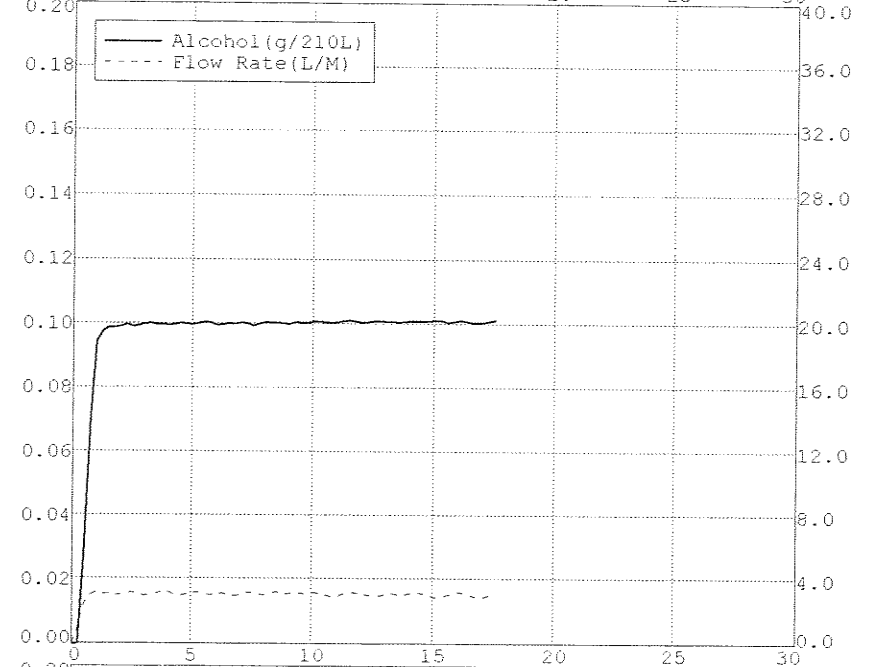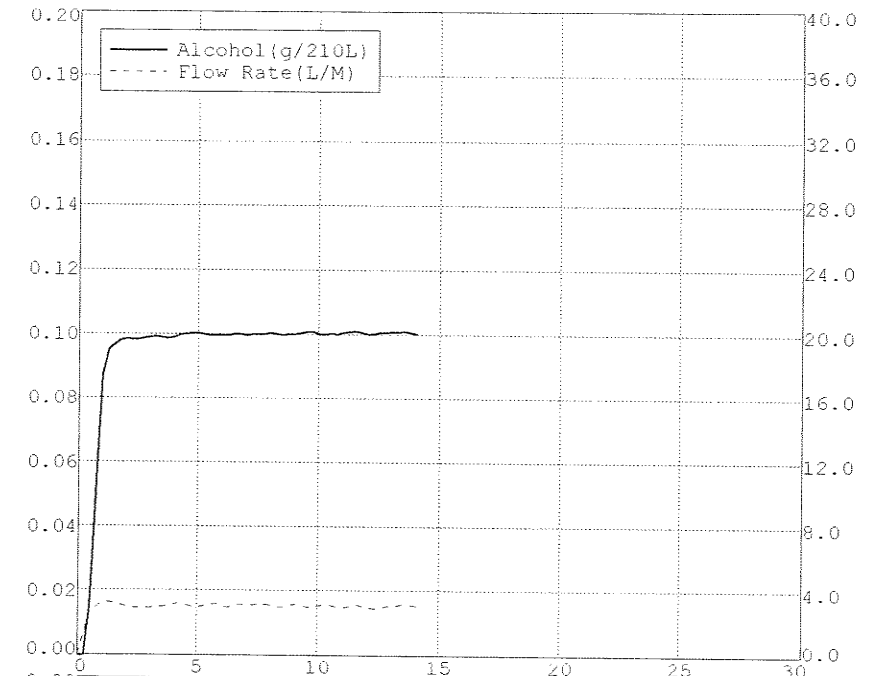

[Handwritten signatures]