

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 06/24/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:02
INTERNAL STANDARD	VERIFIED	11:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:02
BLANK TEST	0.00	11:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:04
BLANK TEST	0.00	11:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:05
BLANK TEST	0.00	11:06

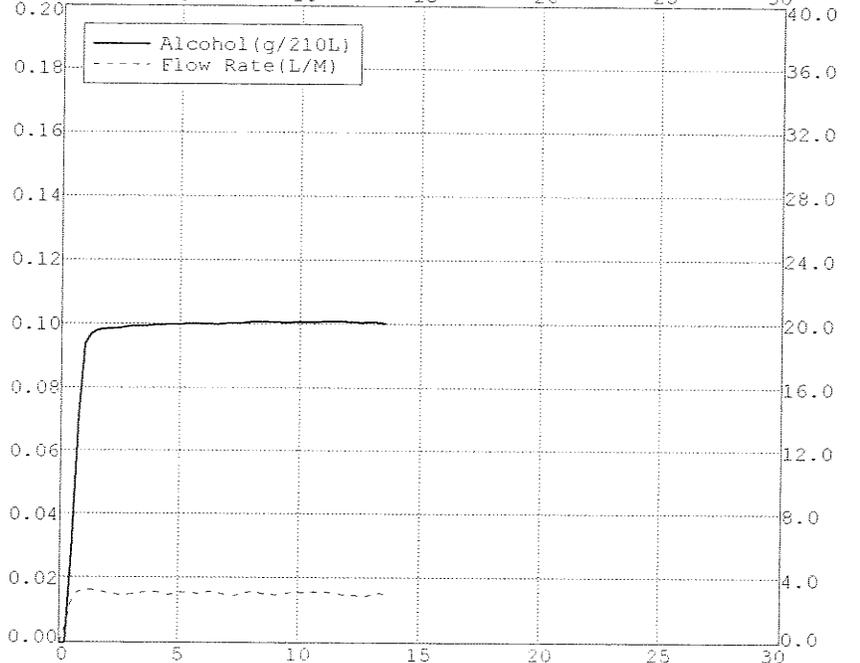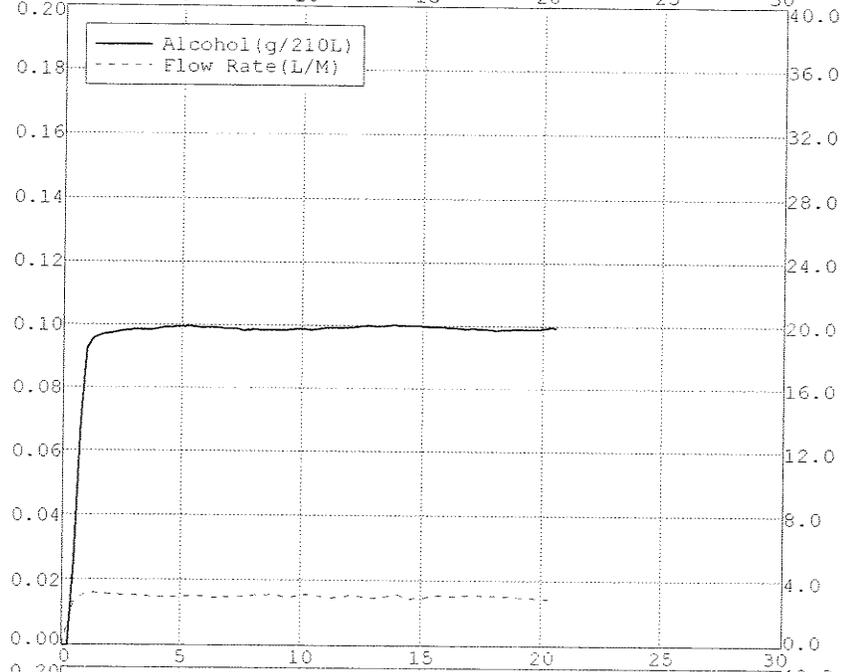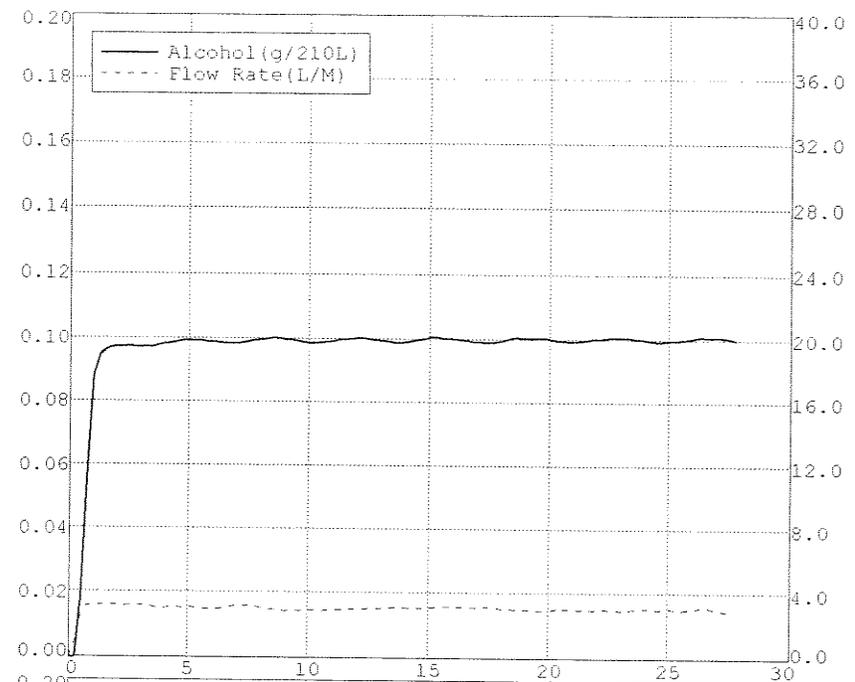

Charles B Geisler #295