

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 07/08/2019

OPERATOR NAME:
TYLER J MORSE
Permit #: 41959
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 12:43 |
| INTERNAL STANDARD | VERIFIED | 12:43 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 12:43 |
| BLANK TEST | 0.00 | 12:44 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 12:45 |
| BLANK TEST | 0.00 | 12:46 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 12:46 |
| BLANK TEST | 0.00 | 12:47 |

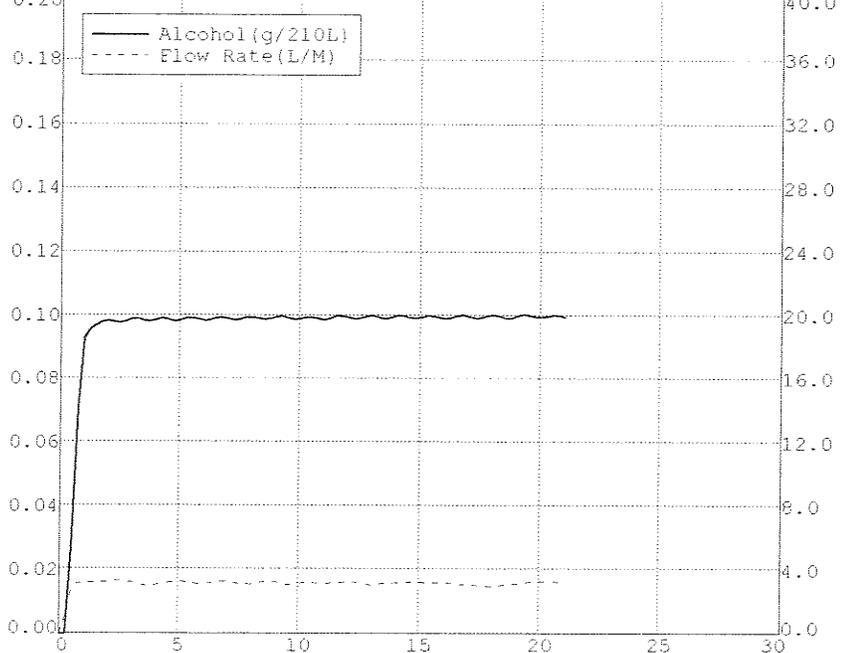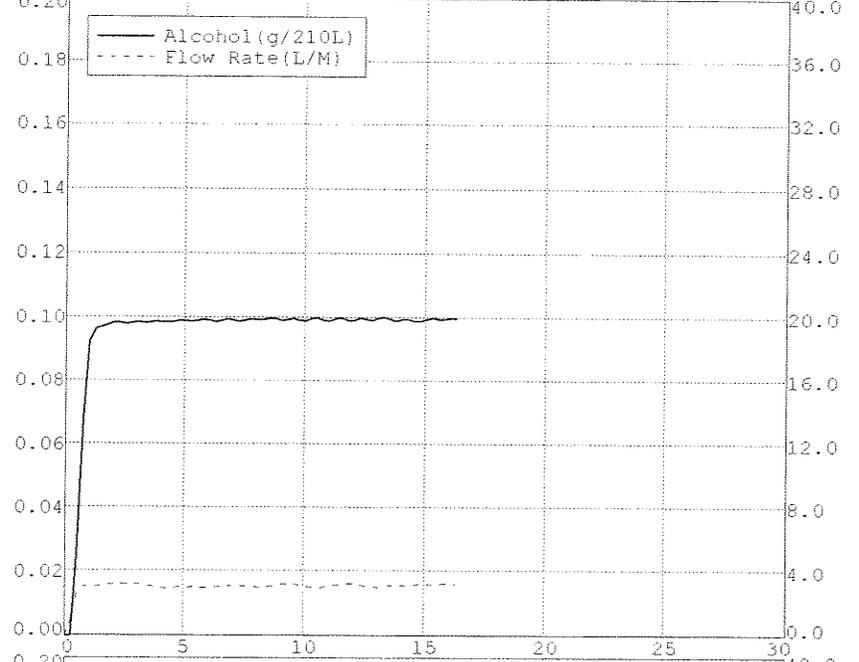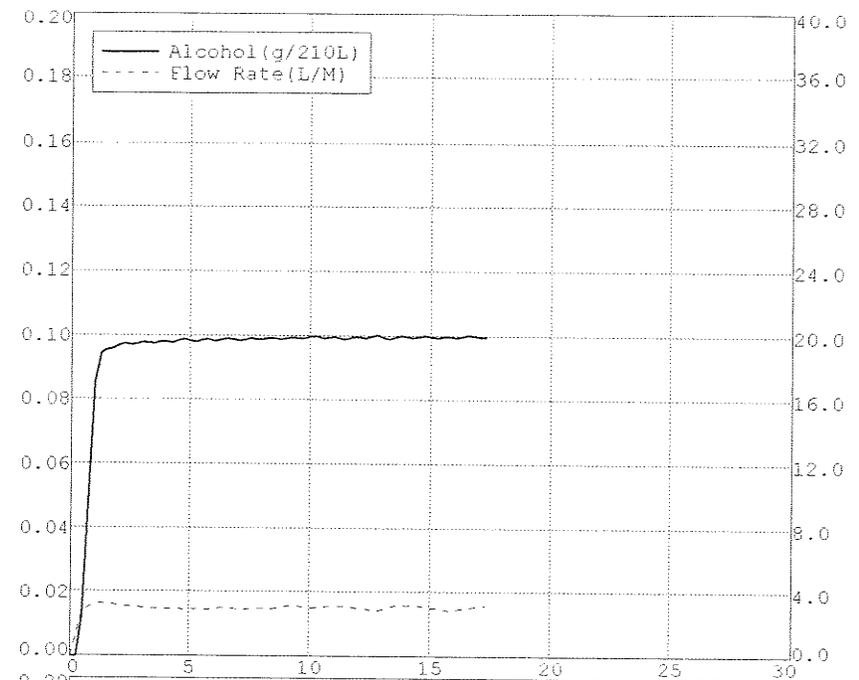

POJ #447