

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 07/29/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:19
INTERNAL STANDARD	VERIFIED	02:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:20
BLANK TEST	0.00	02:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:21
BLANK TEST	0.00	02:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:22
BLANK TEST	0.00	02:23

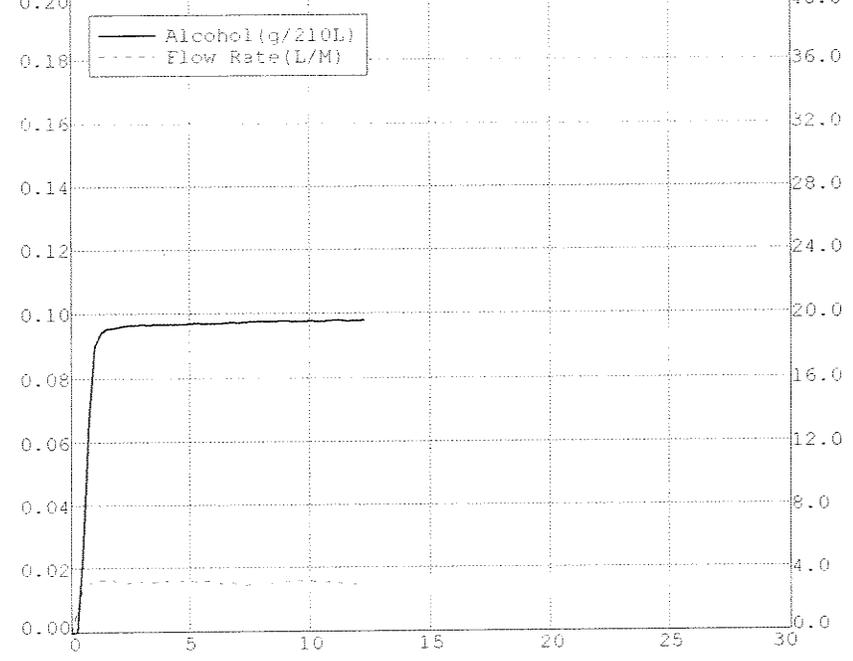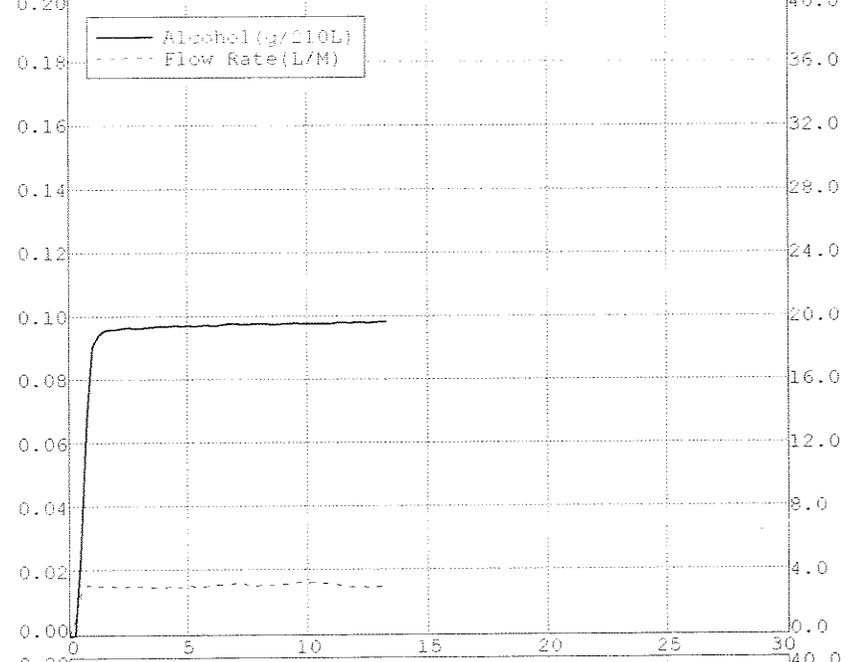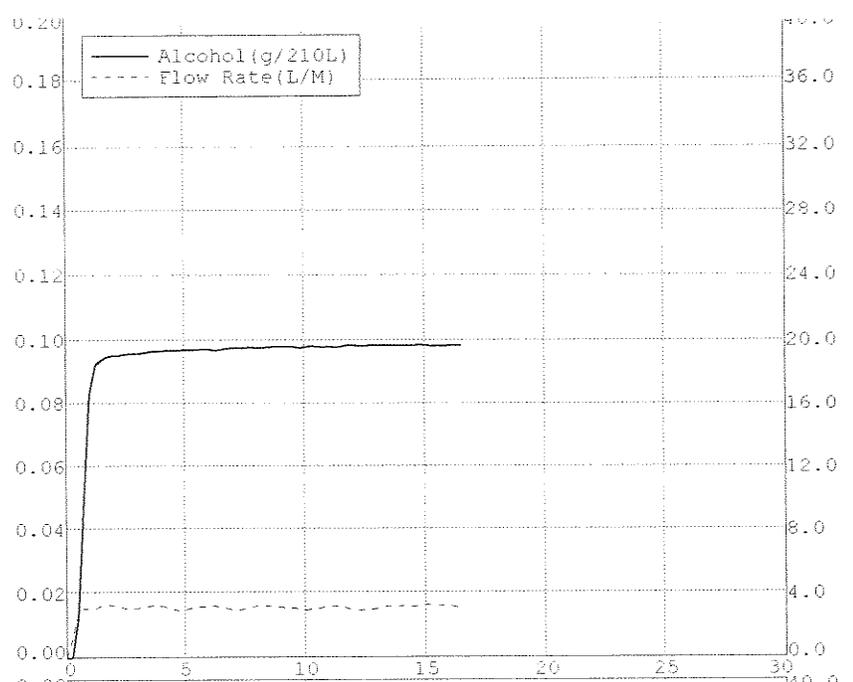

*Signature: Sgt. C. B. Geisler*