

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 08/09/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:41
INTERNAL STANDARD	VERIFIED	20:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	20:41
BLANK TEST	0.00	20:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	20:43
BLANK TEST	0.00	20:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	20:44
BLANK TEST	0.00	20:45

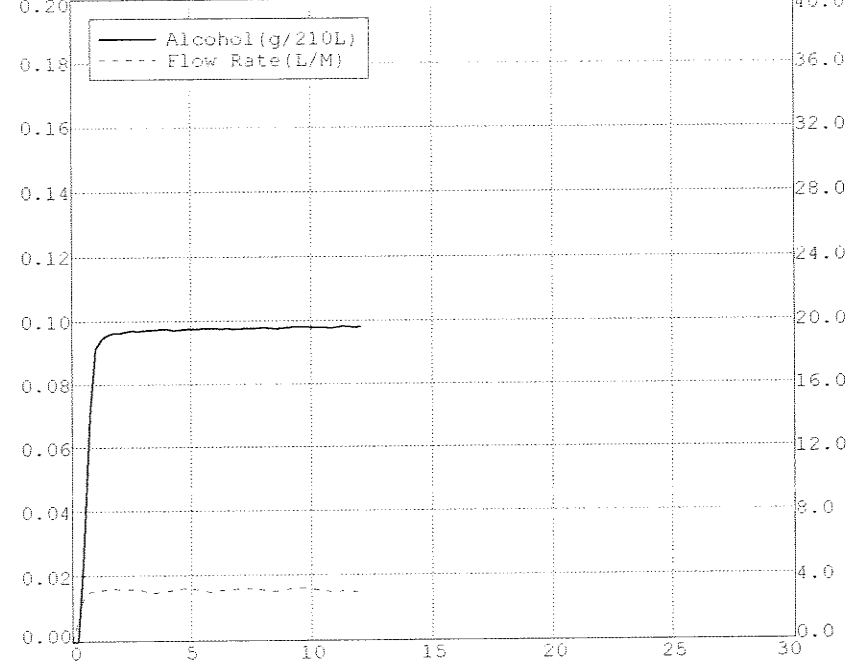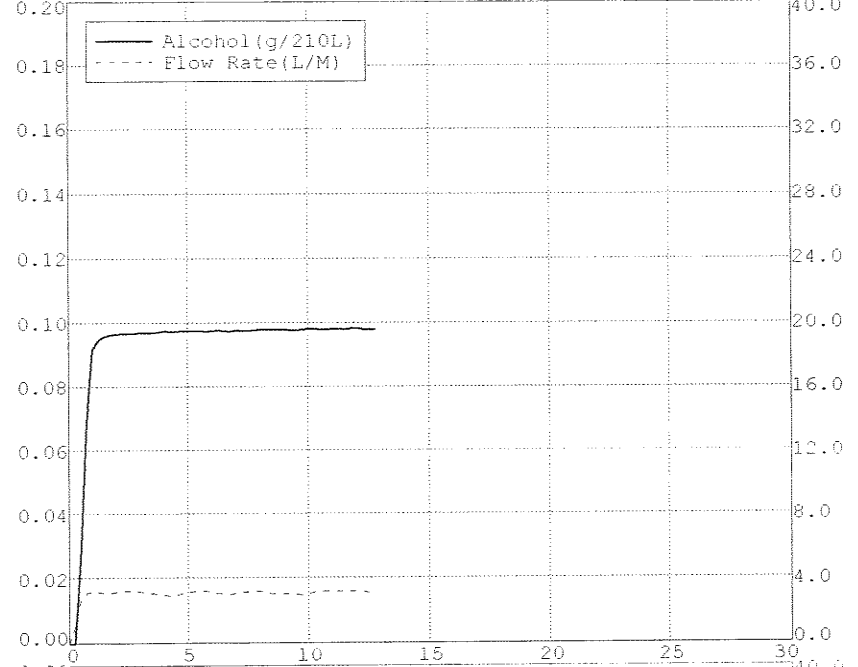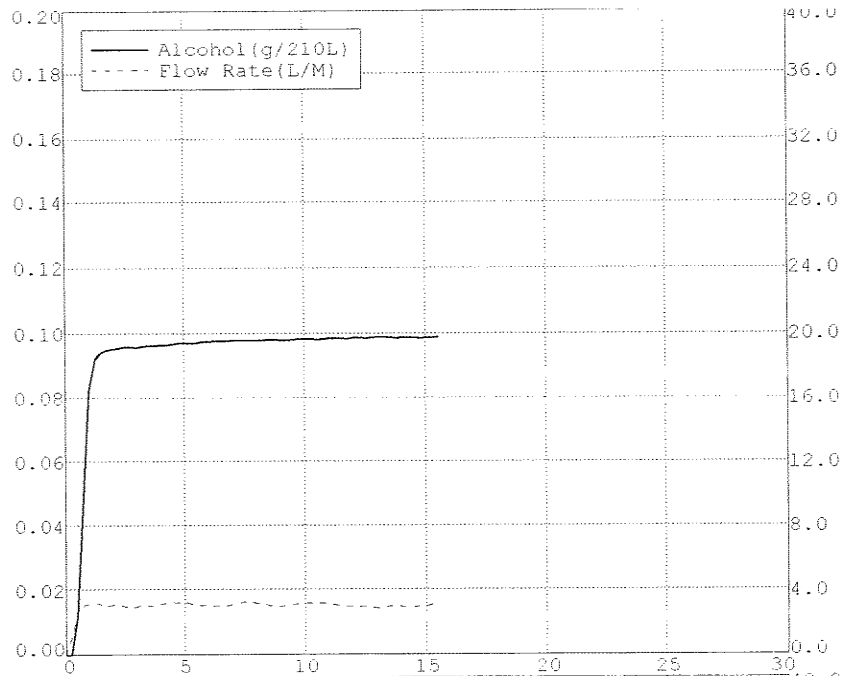

*Sgt. C. B. Geisler*