

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 08/15/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:07
INTERNAL STANDARD	VERIFIED	04:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:08
BLANK TEST	0.00	04:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:09
BLANK TEST	0.00	04:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:10
BLANK TEST	0.00	04:11

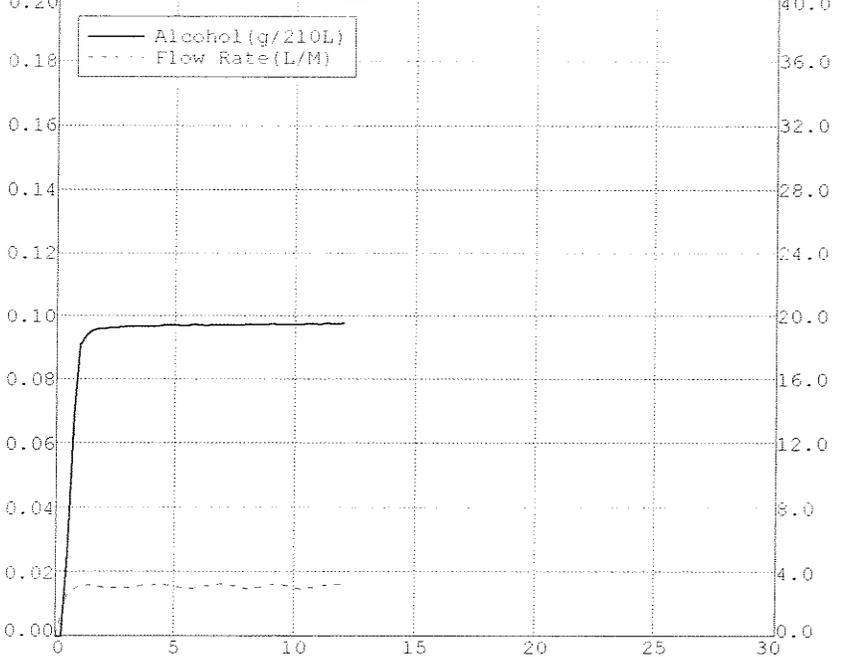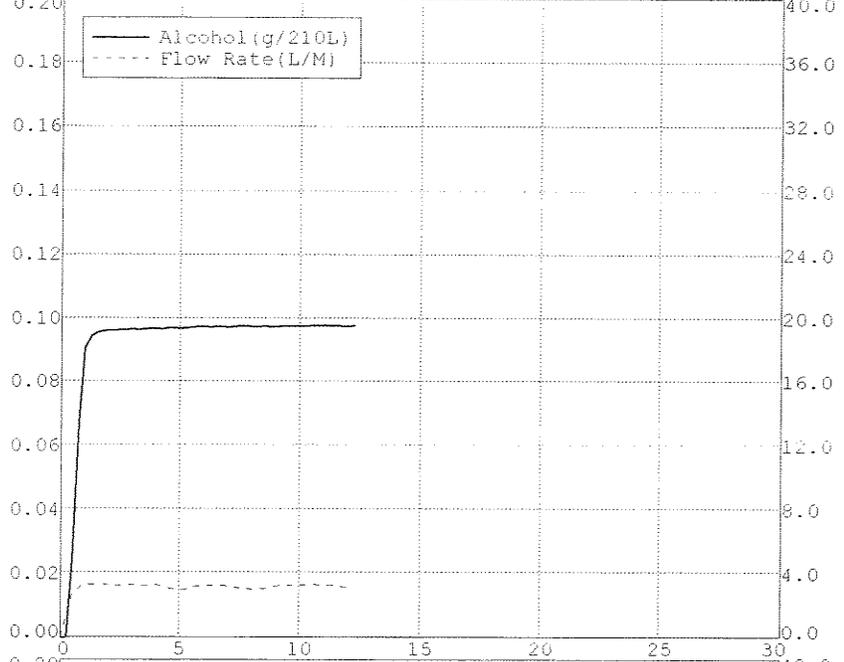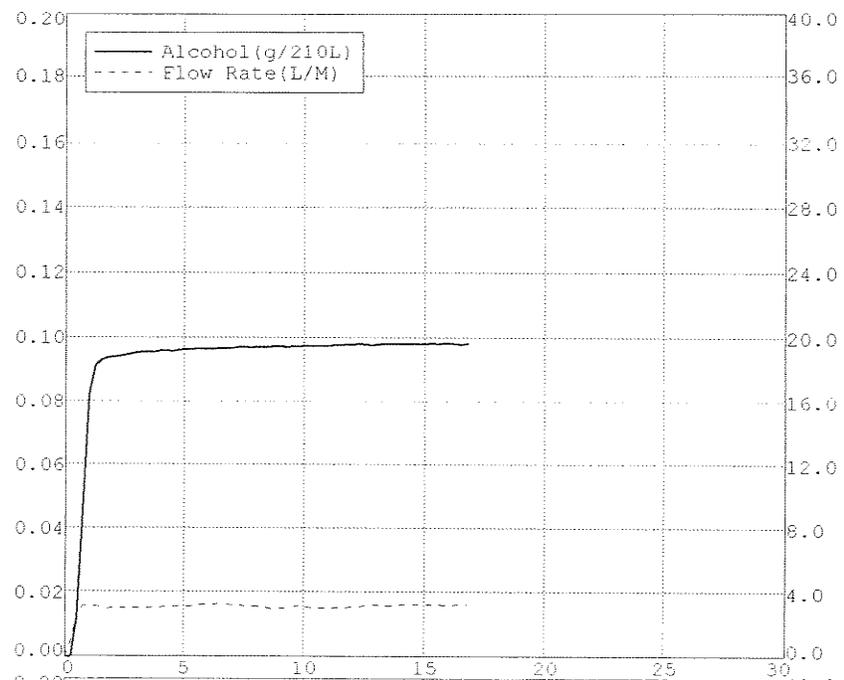

Handwritten signatures and initials:
C. B. Geisler
#2