

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 08/20/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:45
INTERNAL STANDARD	VERIFIED	18:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:45
BLANK TEST	0.00	18:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:46
BLANK TEST	0.00	18:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:48
BLANK TEST	0.00	18:49

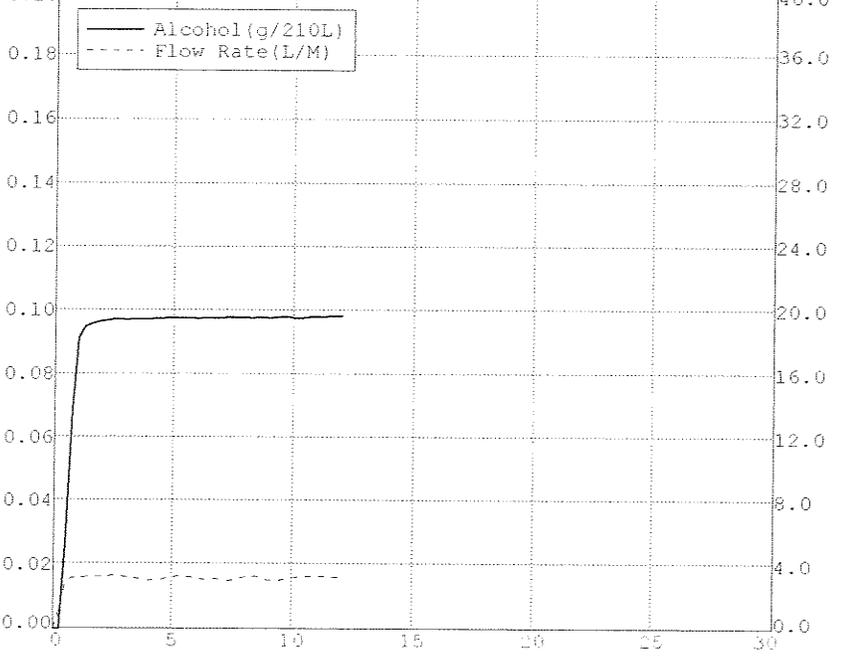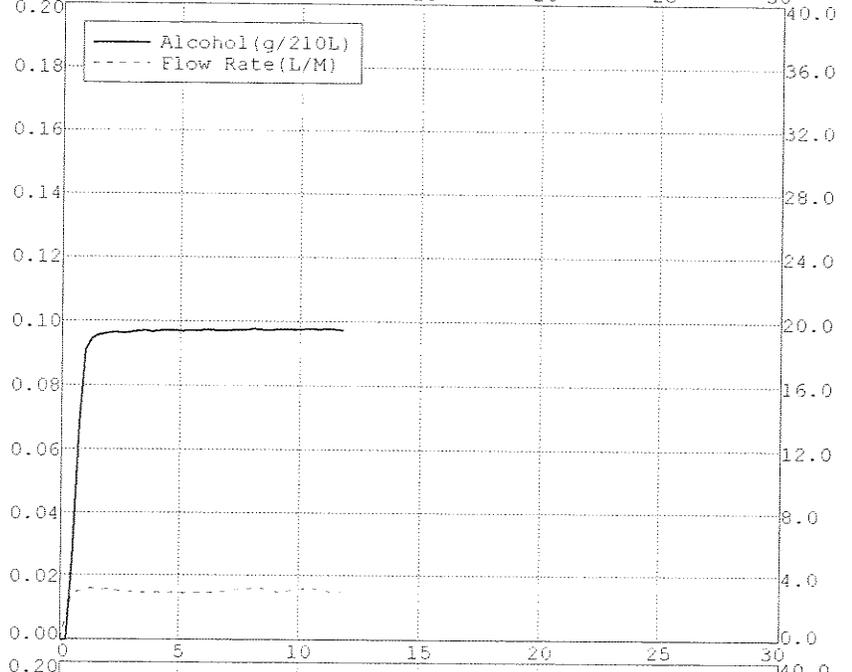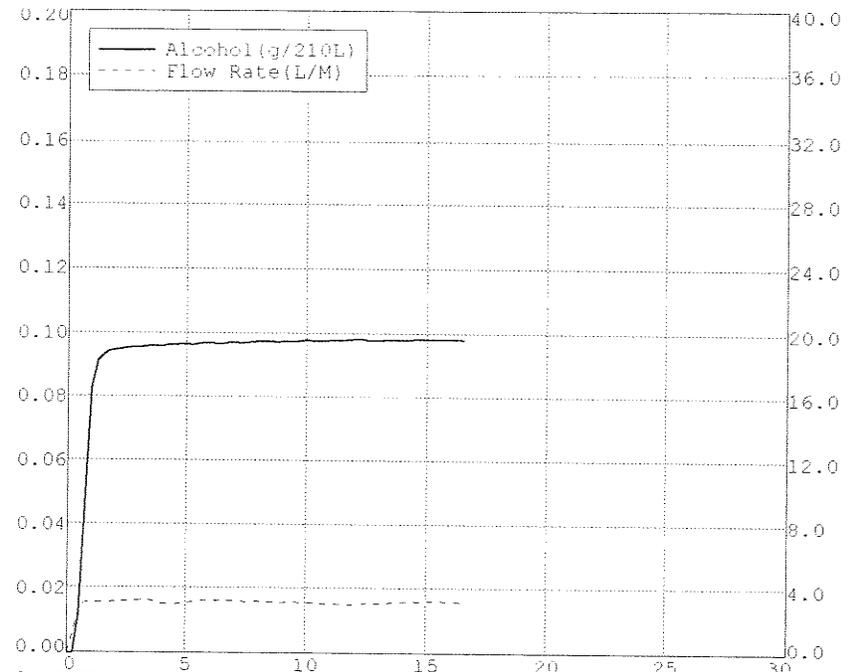

*Charles B. Geisler*