

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 08/27/2019

OPERATOR NAME:  
J T COON  
Permit #: 36043  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:27
INTERNAL STANDARD	VERIFIED	06:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:28
BLANK TEST	0.00	06:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:29
BLANK TEST	0.00	06:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:30
BLANK TEST	0.00	06:31

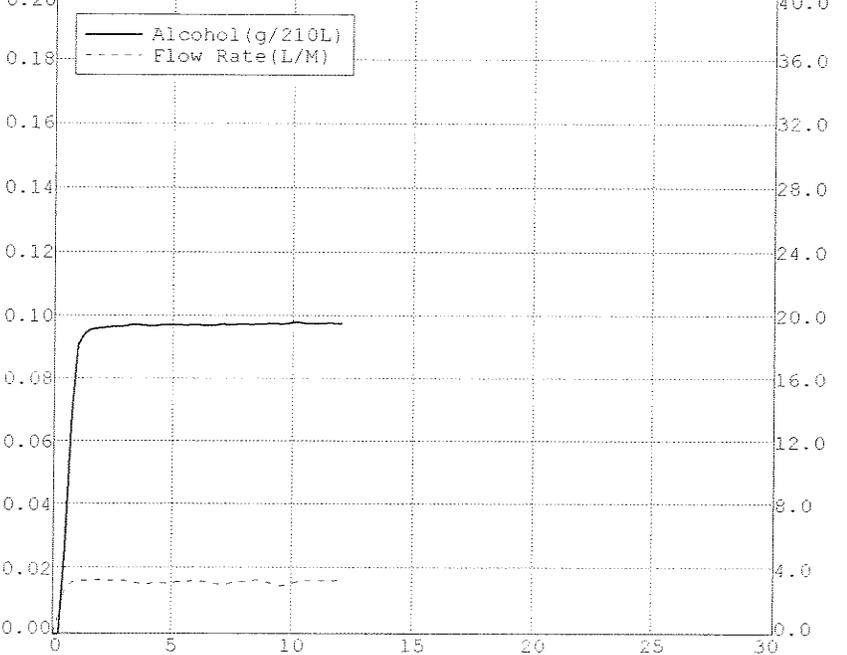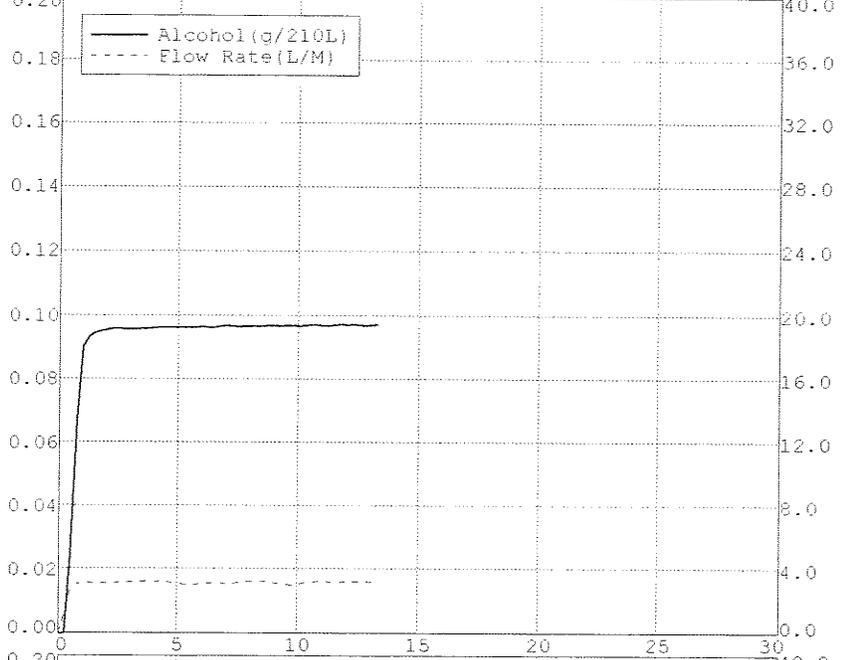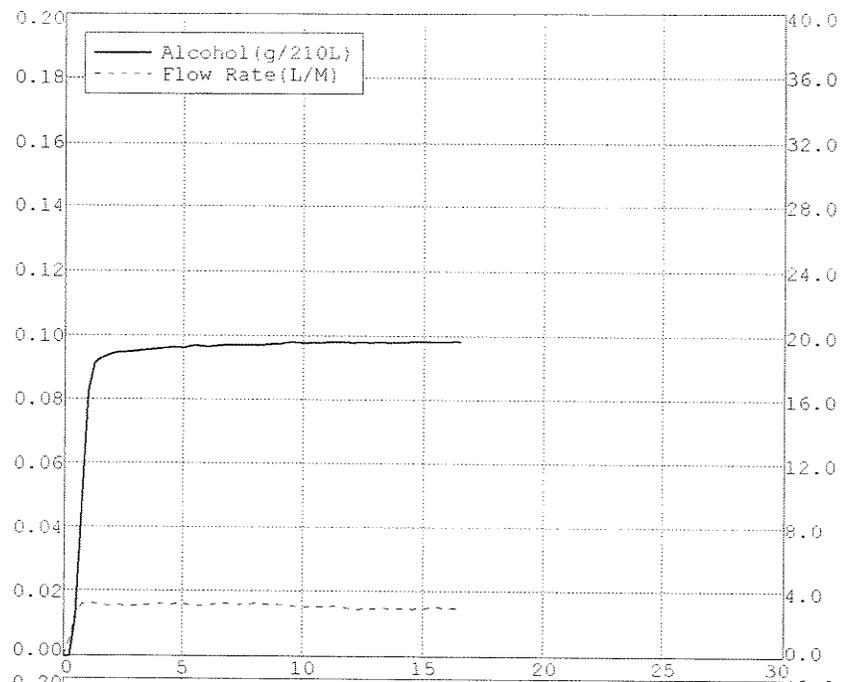

*P.O. [Signature]* 321