

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 09/21/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:13
INTERNAL STANDARD	VERIFIED	06:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:13
BLANK TEST	0.00	06:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:14
BLANK TEST	0.00	06:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:16
BLANK TEST	0.00	06:16

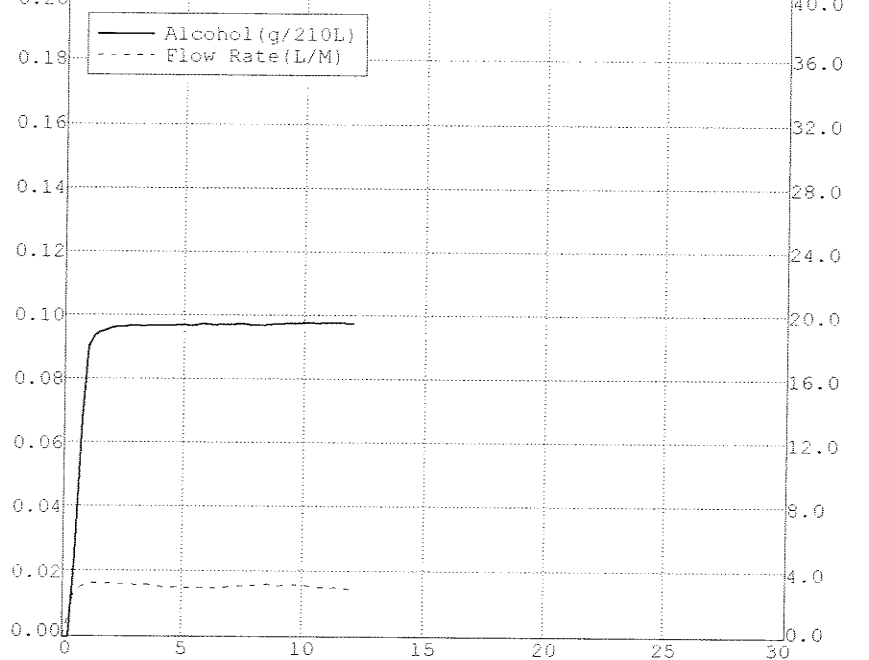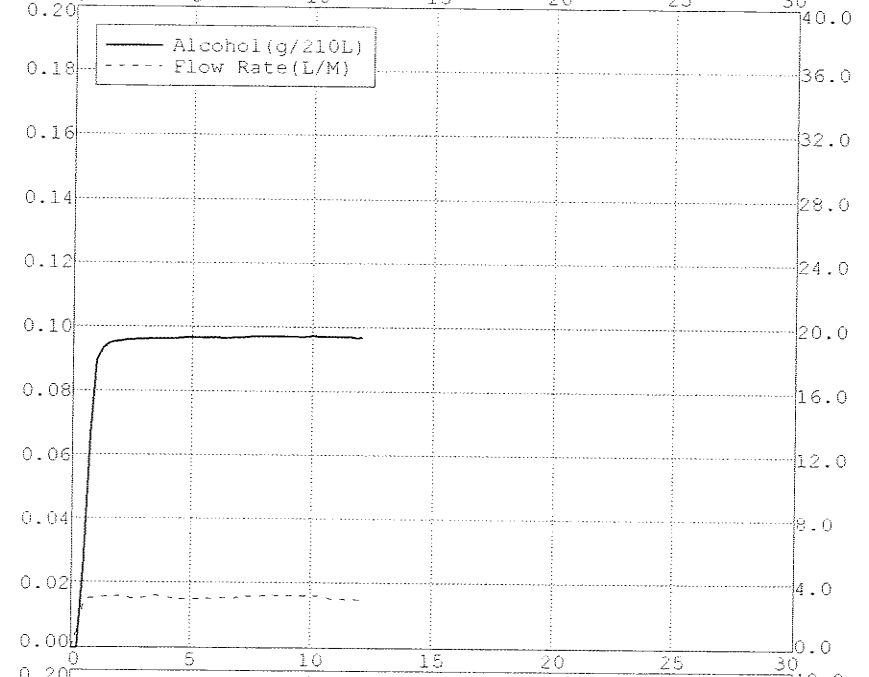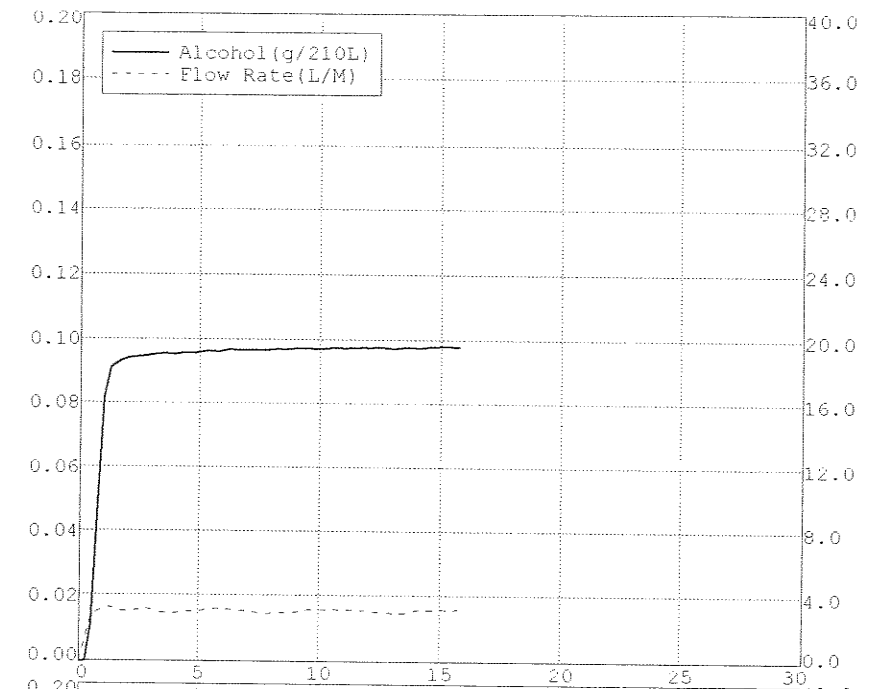

Charles B. Geisler #2w