

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 10/16/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:18
INTERNAL STANDARD	VERIFIED	00:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:19
BLANK TEST	0.00	00:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:20
BLANK TEST	0.00	00:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:21
BLANK TEST	0.00	00:22

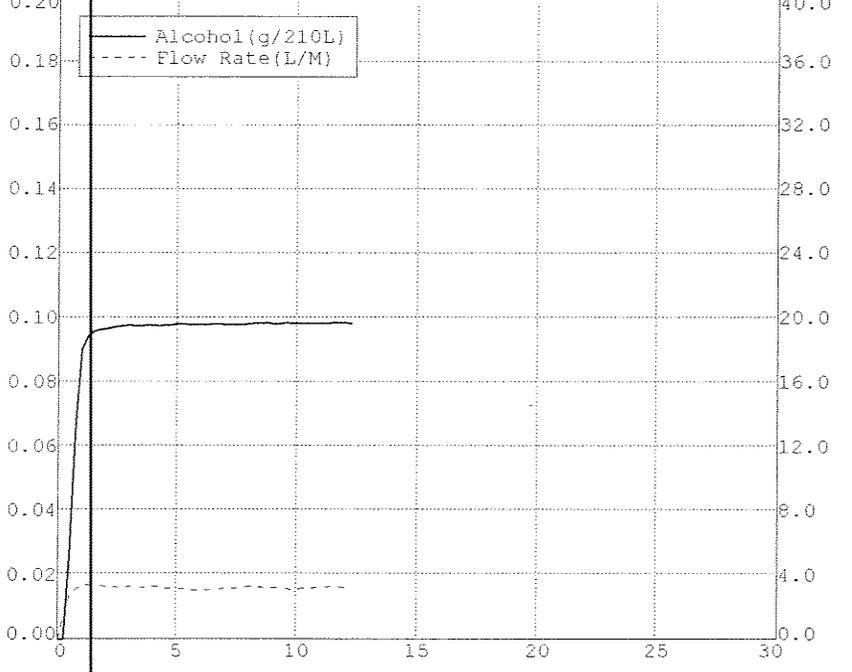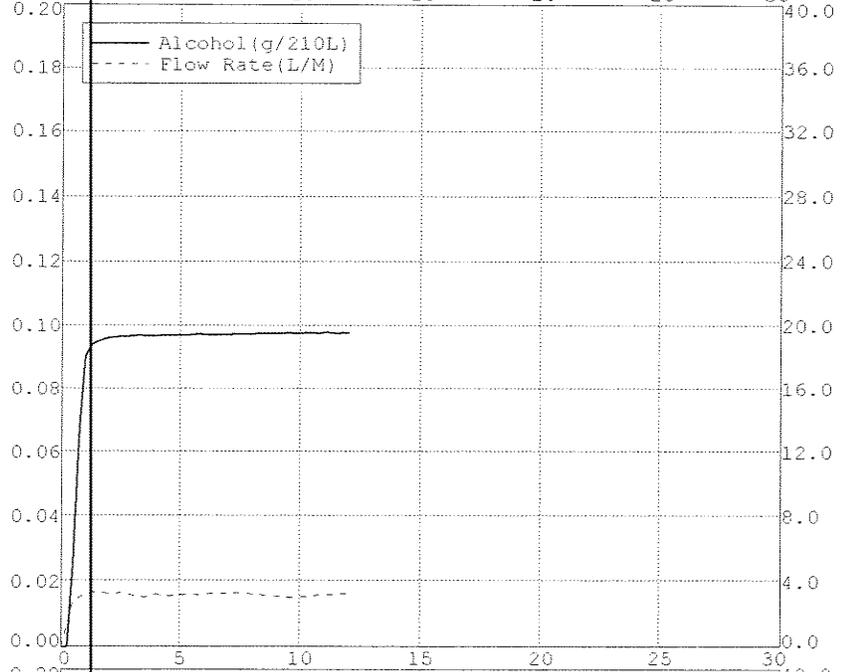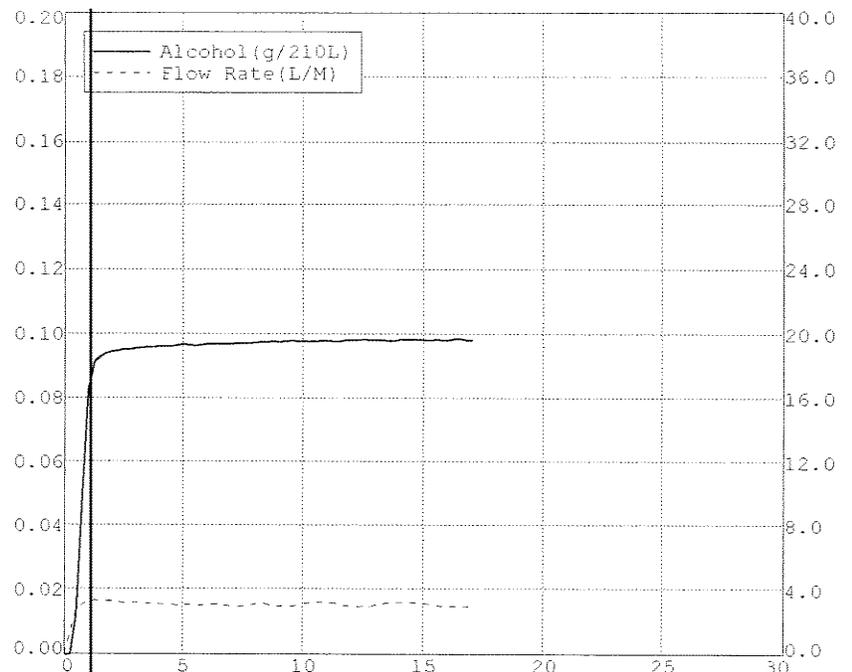

Ch. B. Geisler #244