

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 10/24/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:20
INTERNAL STANDARD	VERIFIED	00:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:21
BLANK TEST	0.00	00:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:22
BLANK TEST	0.00	00:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:23
BLANK TEST	0.00	00:24

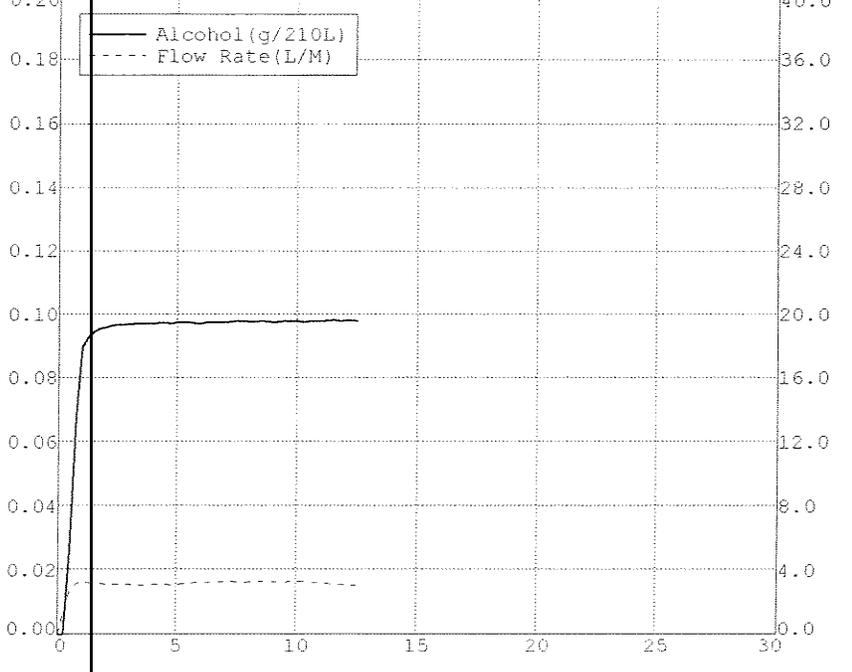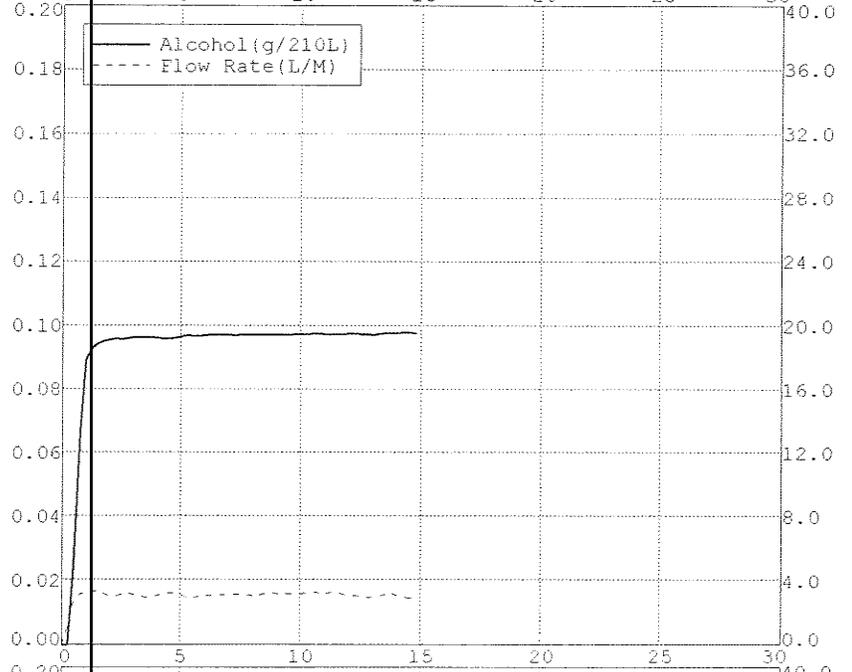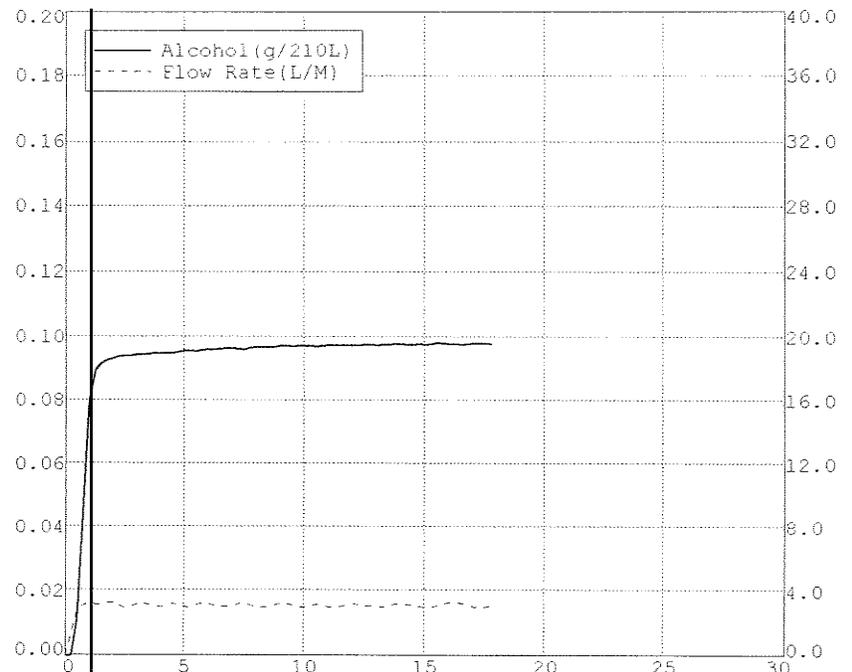

*Charles B. Geisler #210*