

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 11/07/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:31
INTERNAL STANDARD	VERIFIED	11:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:32
BLANK TEST	0.00	11:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:33
BLANK TEST	0.00	11:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:34
BLANK TEST	0.00	11:35

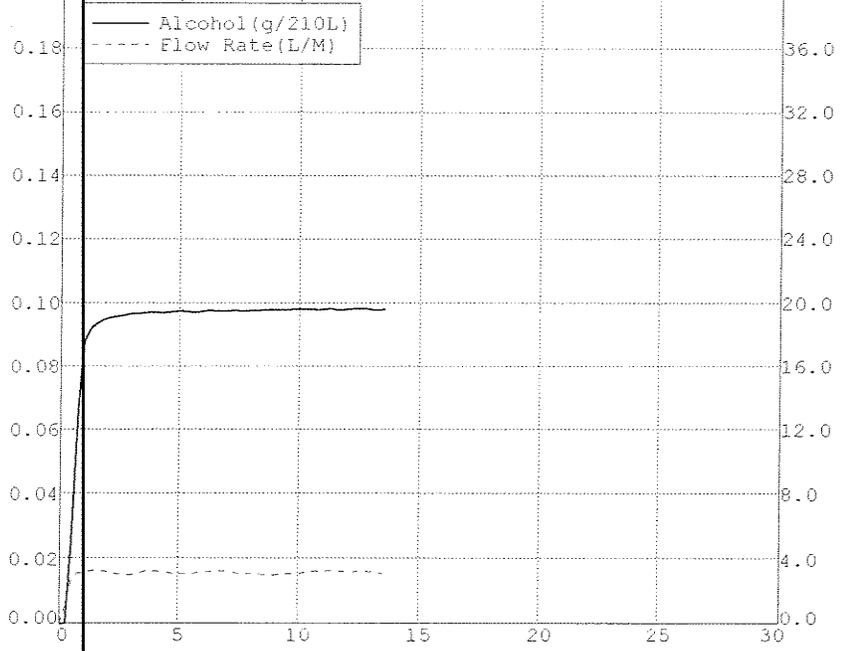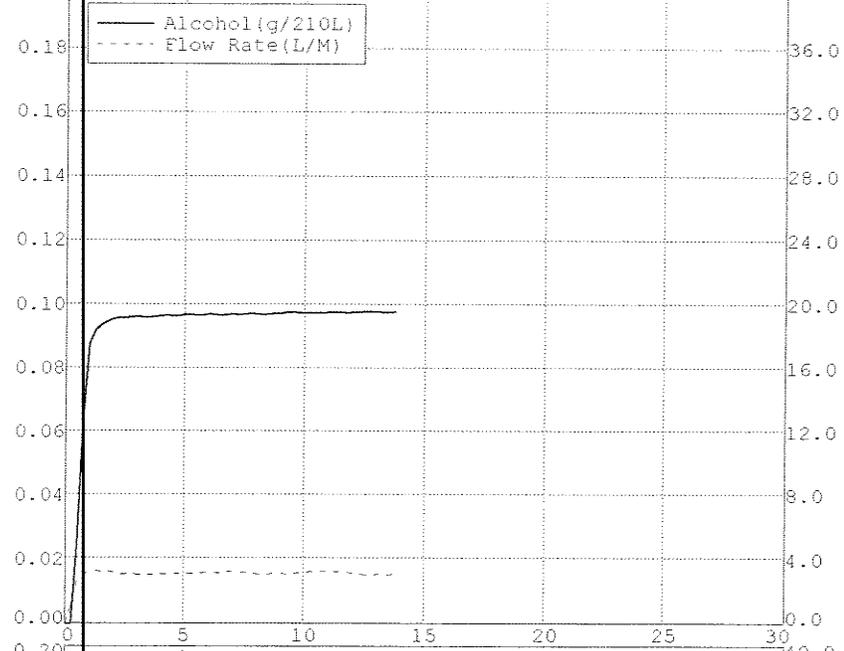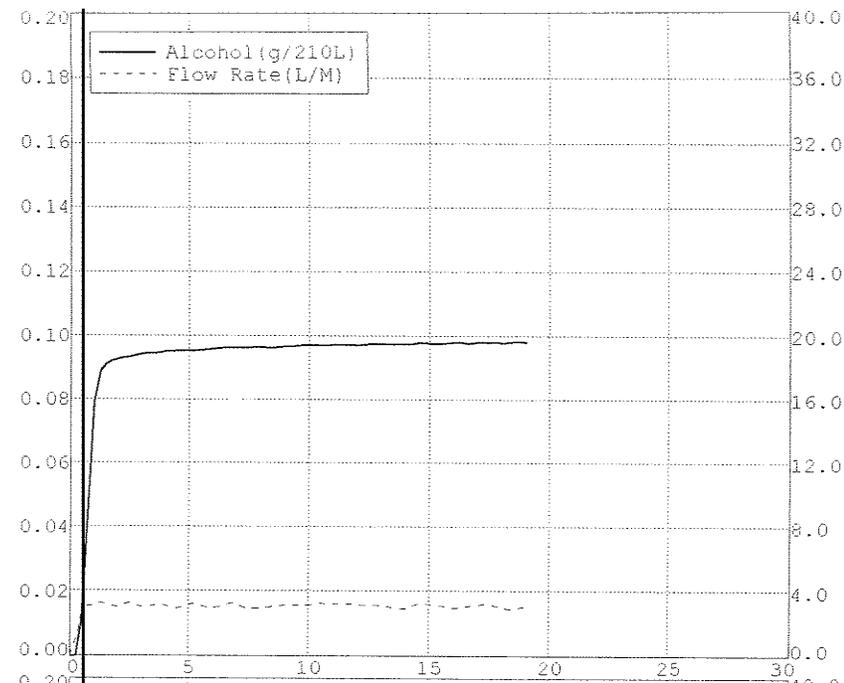

*Signature: Sgt. Charles B. Geisler*  
#20