

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 11/16/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:28
INTERNAL STANDARD	VERIFIED	00:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:28
BLANK TEST	0.00	00:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:29
BLANK TEST	0.00	00:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:30
BLANK TEST	0.00	00:31

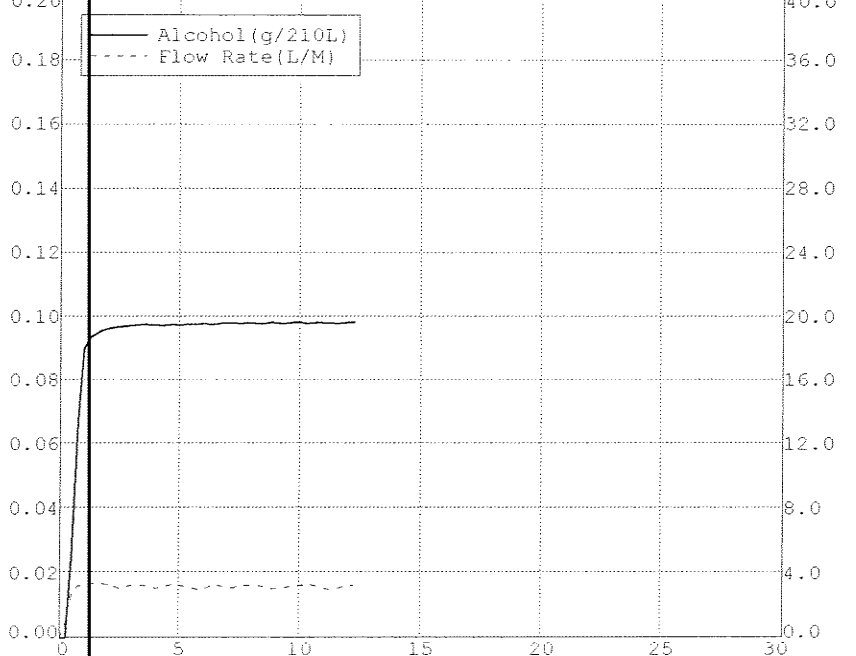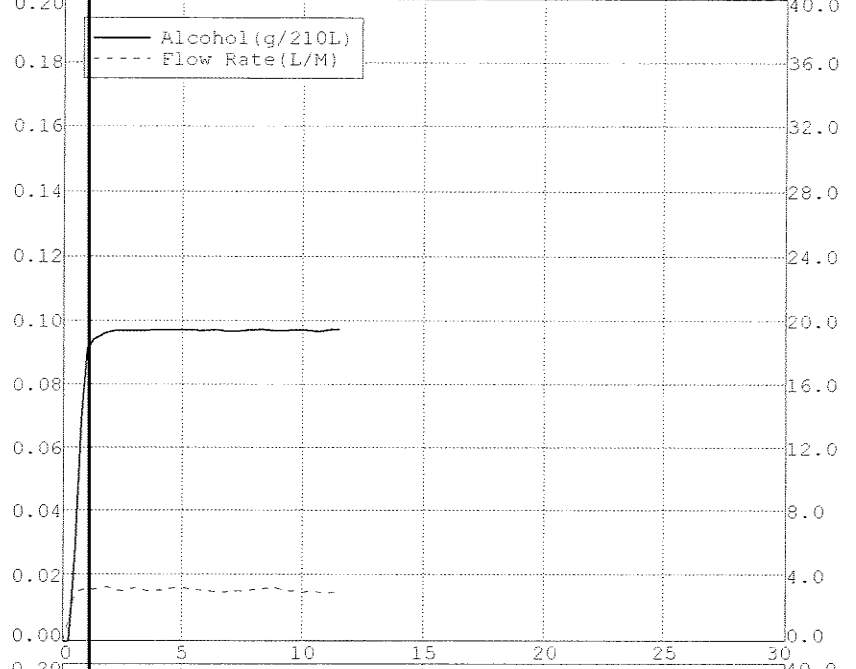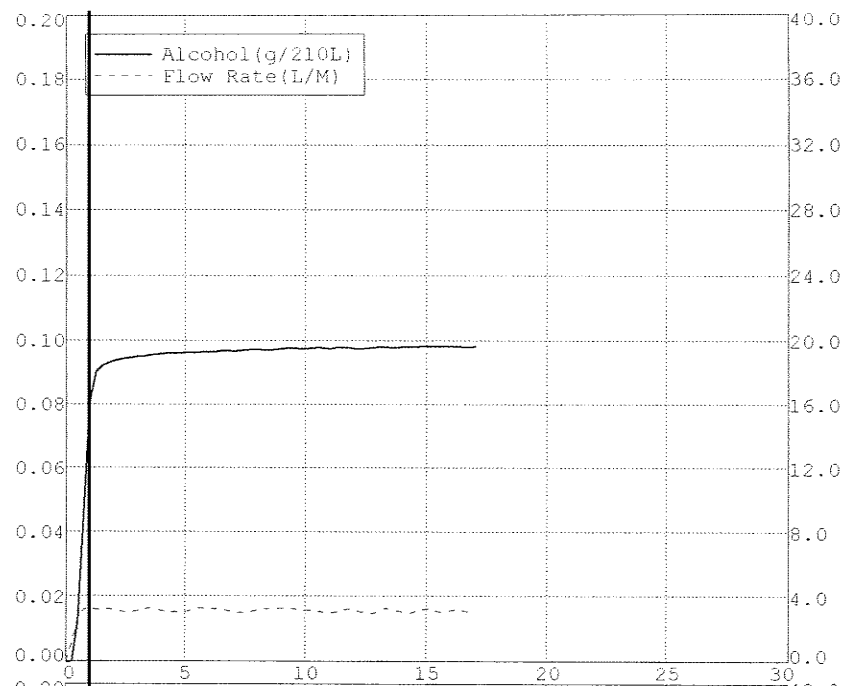

*Handwritten signatures and initials:*  
Sgt. [Signature] [Signature] [Signature]