

SOLUTION CHANGE




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 12/01/2019

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:54
INTERNAL STANDARD	VERIFIED	01:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:55
BLANK TEST	0.00	01:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:56
BLANK TEST	0.00	01:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:57
BLANK TEST	0.00	01:58

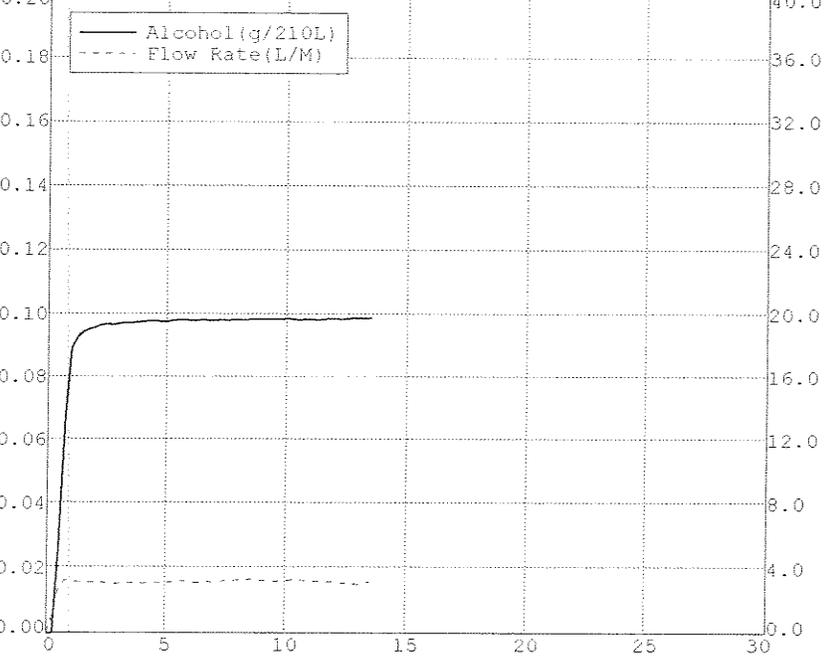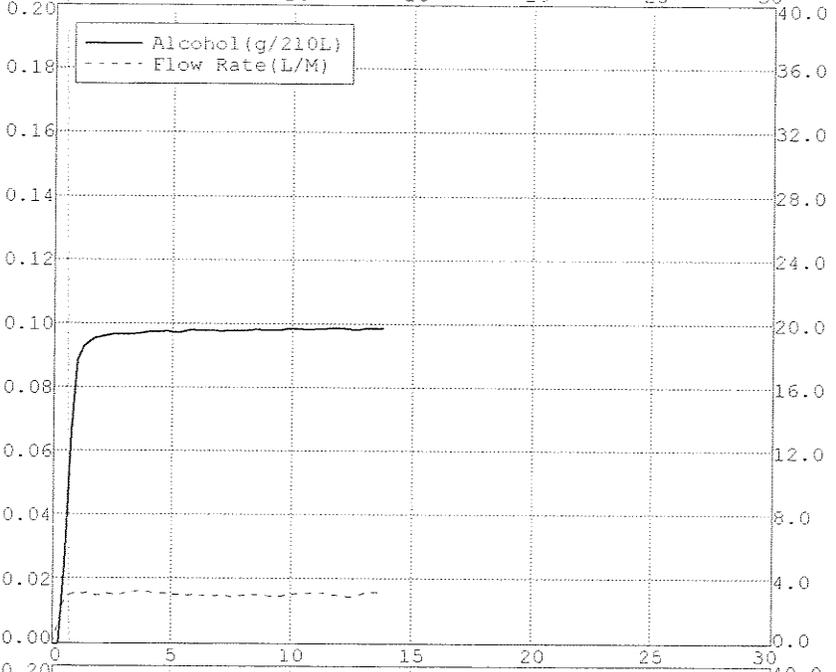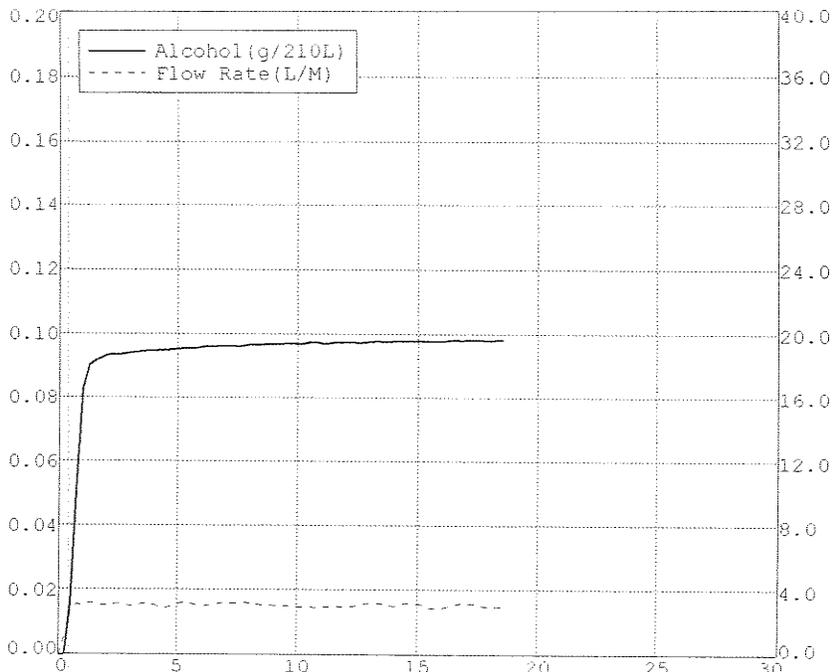

Handwritten signature and initials #241