

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 12/14/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:40
INTERNAL STANDARD	VERIFIED	06:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:41
BLANK TEST	0.00	06:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:42
BLANK TEST	0.00	06:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:43
BLANK TEST	0.00	06:44

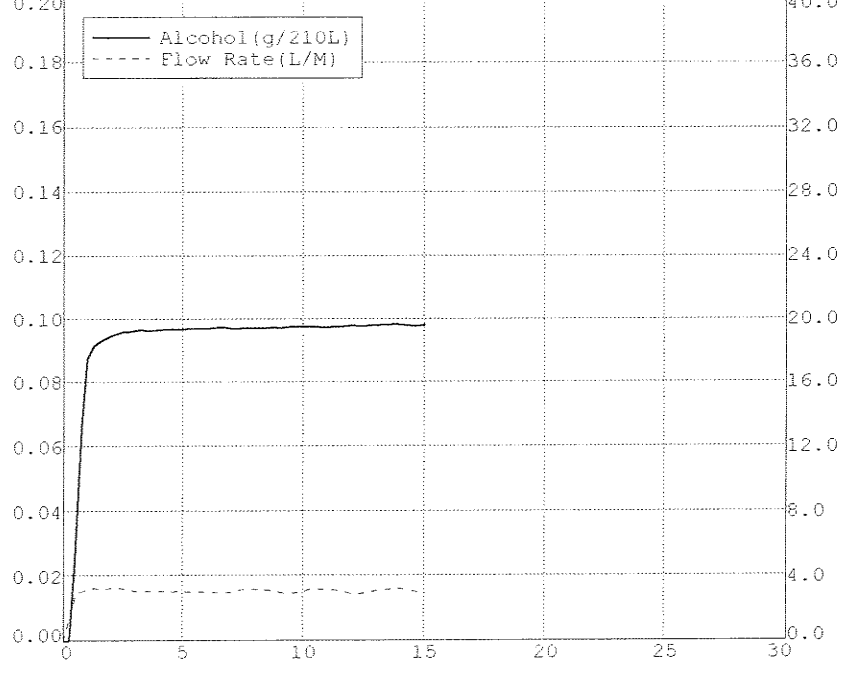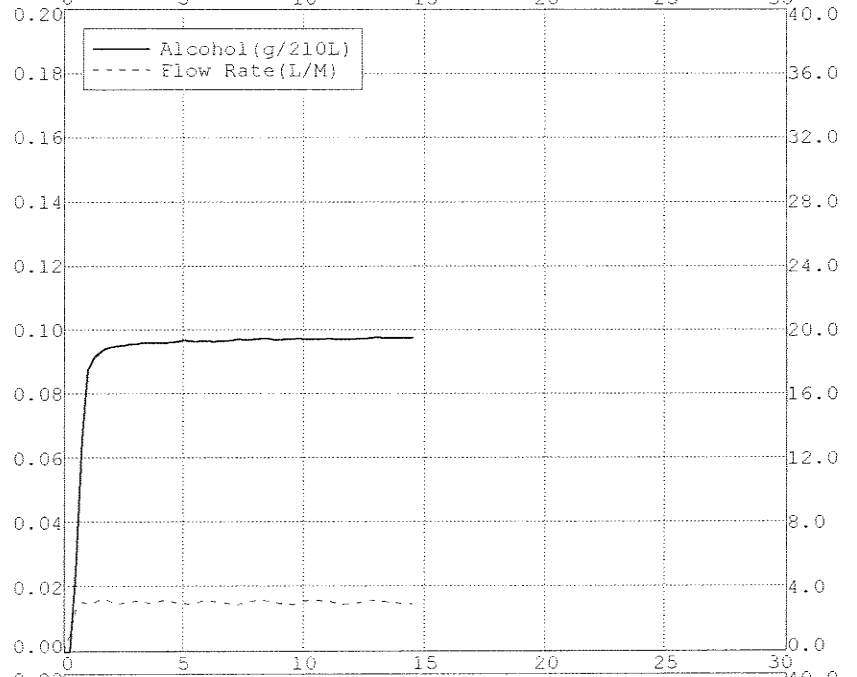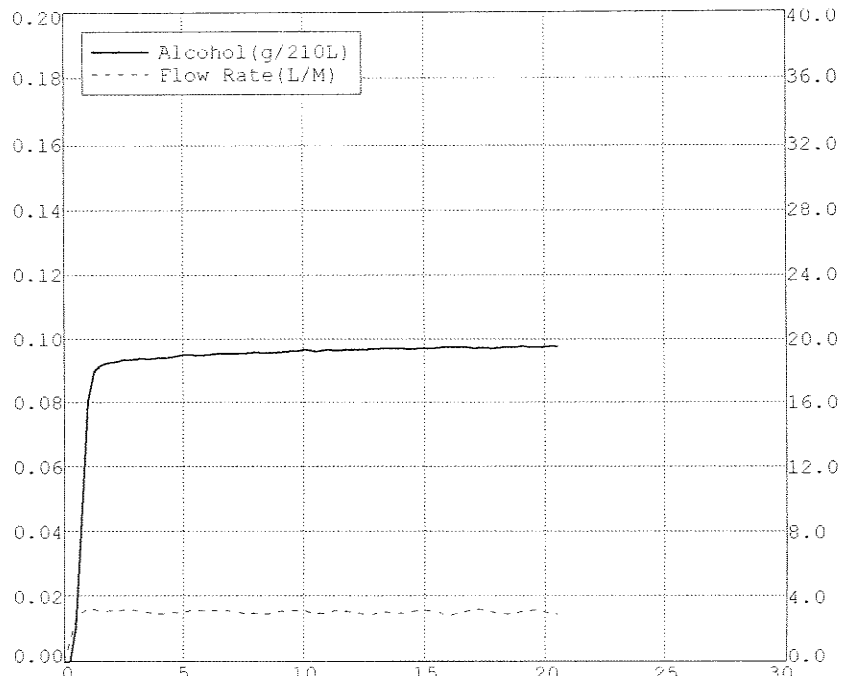

Handwritten signatures and initials:
G.A. [Signature] [Signature] [Signature] H [Signature]