

SUPERVISOR TEST




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 106606

Date: 12/21/2019

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:29
INTERNAL STANDARD	VERIFIED	01:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:29
BLANK TEST	0.00	01:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:30
BLANK TEST	0.00	01:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:32
BLANK TEST	0.00	01:33

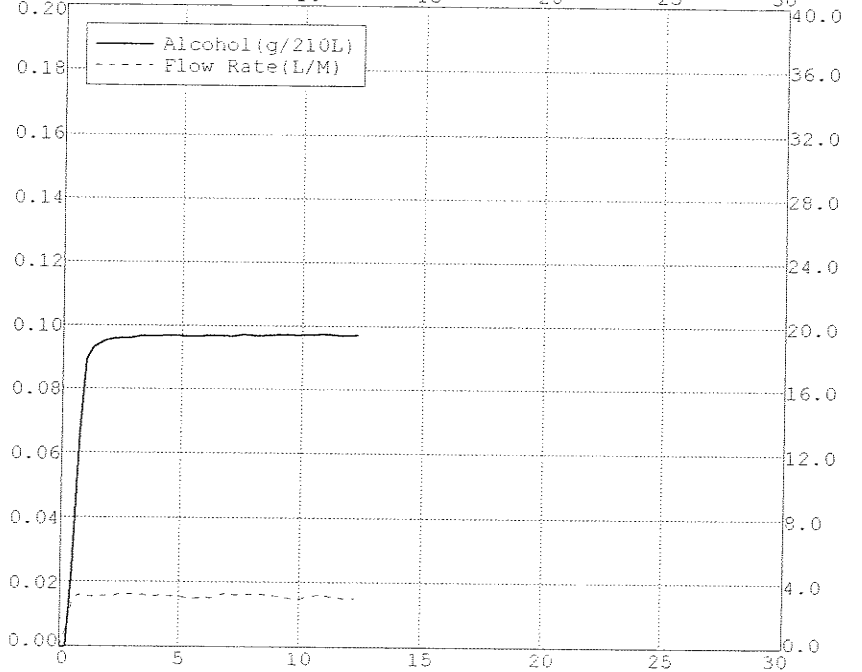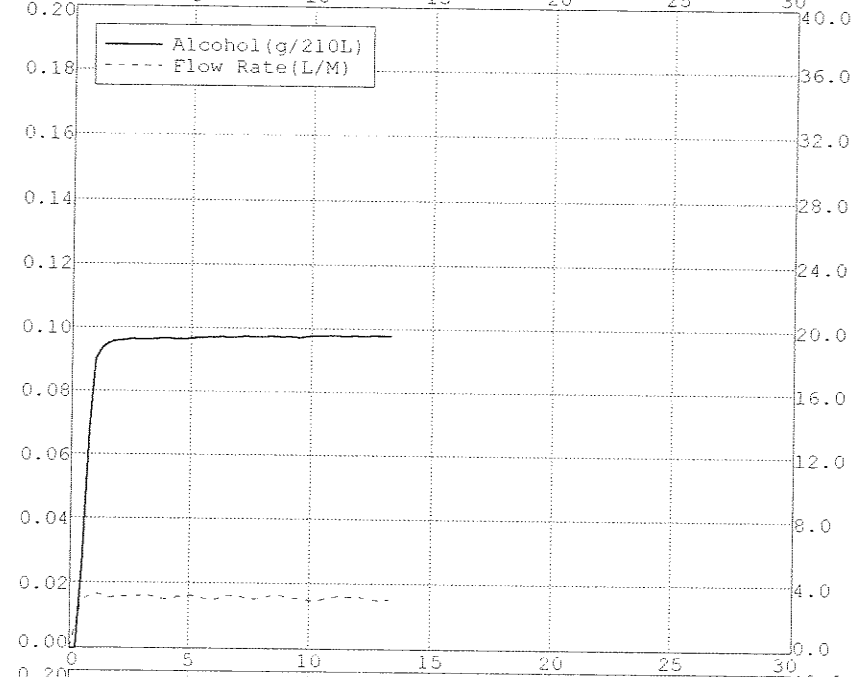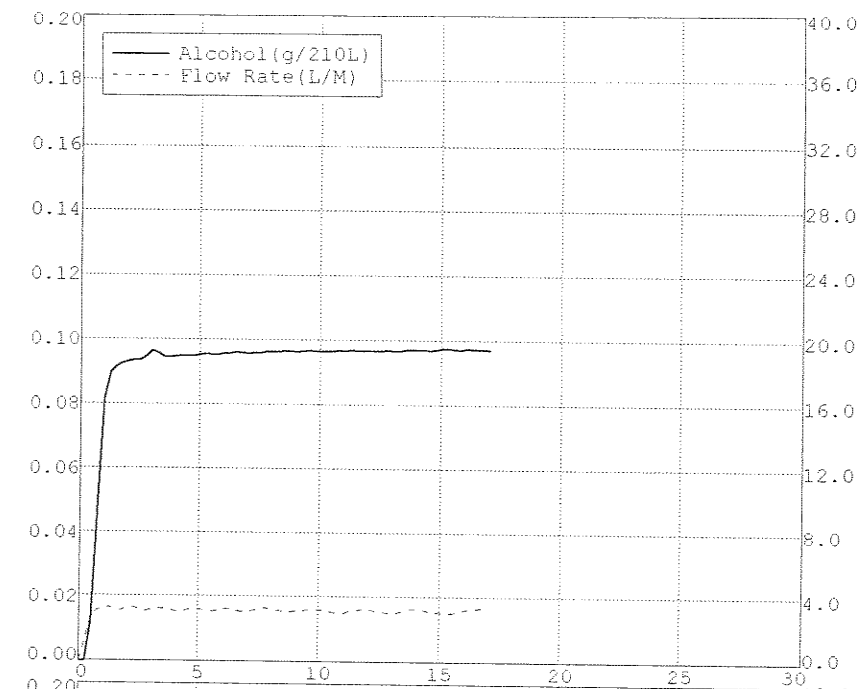

*Sgt. Charles B. Geisler #246*