

SOLUTION CHANGE




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 01/02/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:05
INTERNAL STANDARD	VERIFIED	22:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:06
BLANK TEST	0.00	22:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:07
BLANK TEST	0.00	22:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:08
BLANK TEST	0.00	22:09

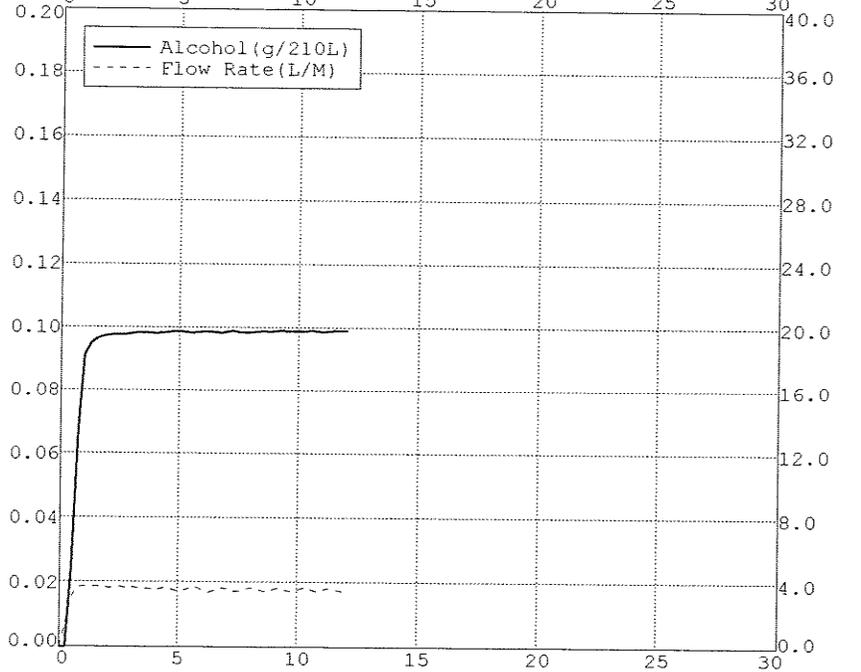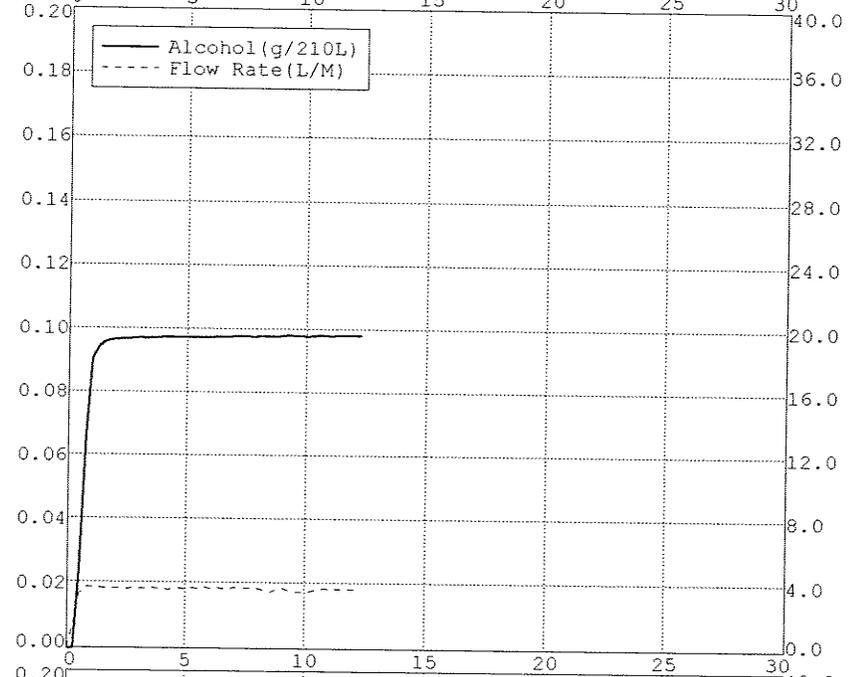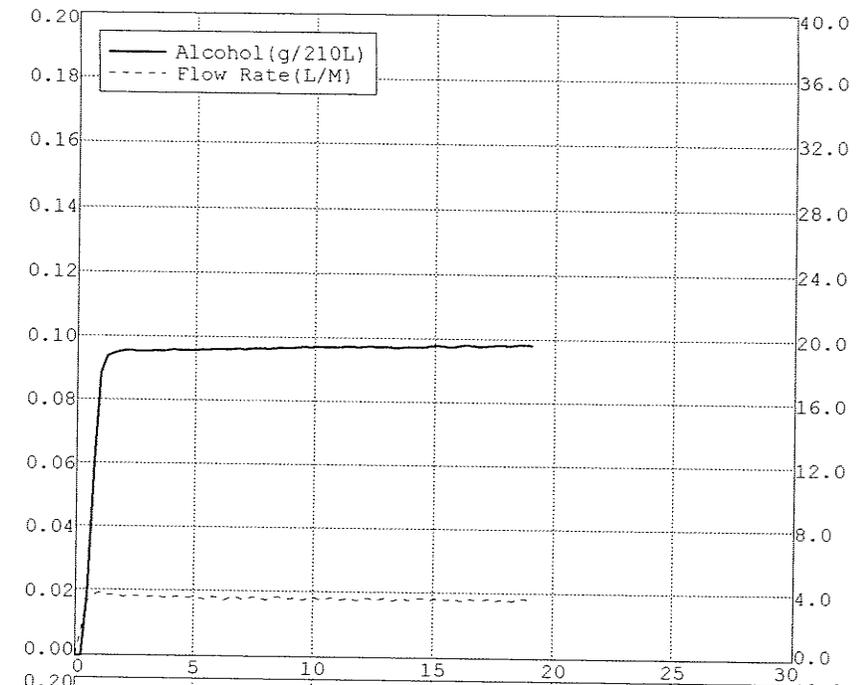

Charles B. Geisler #248