

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 01/07/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:56
INTERNAL STANDARD	VERIFIED	21:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:56
BLANK TEST	0.00	21:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:58
BLANK TEST	0.00	21:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:59
BLANK TEST	0.00	22:00

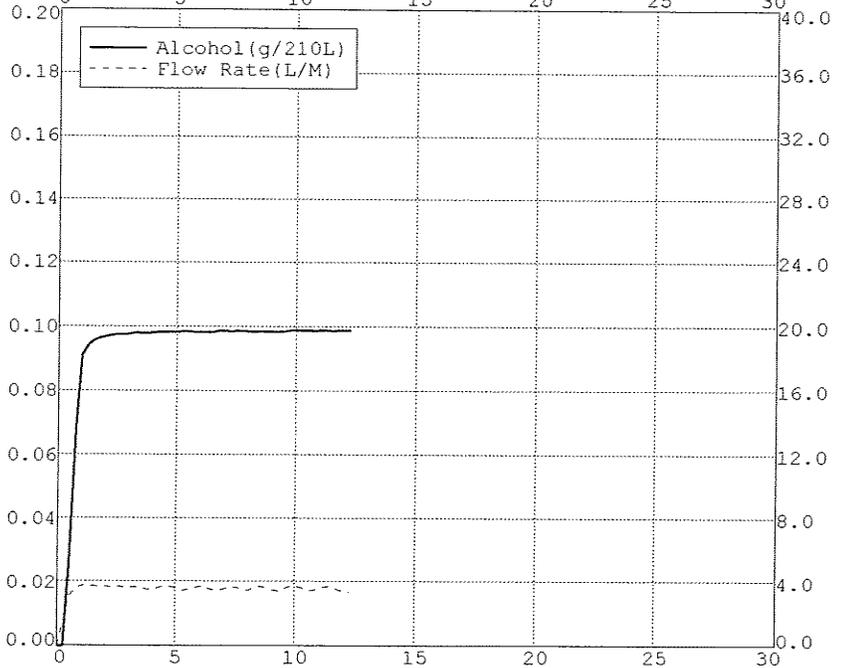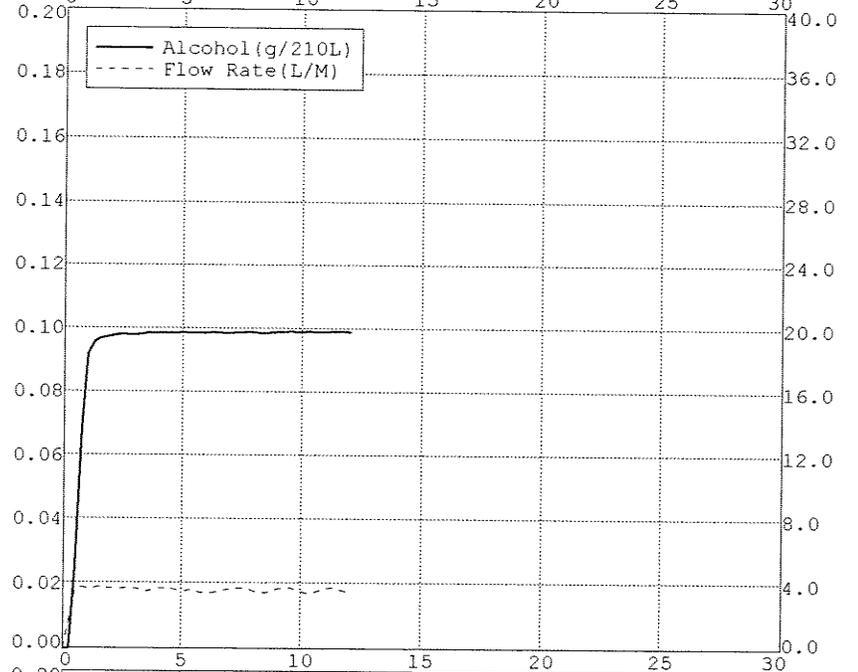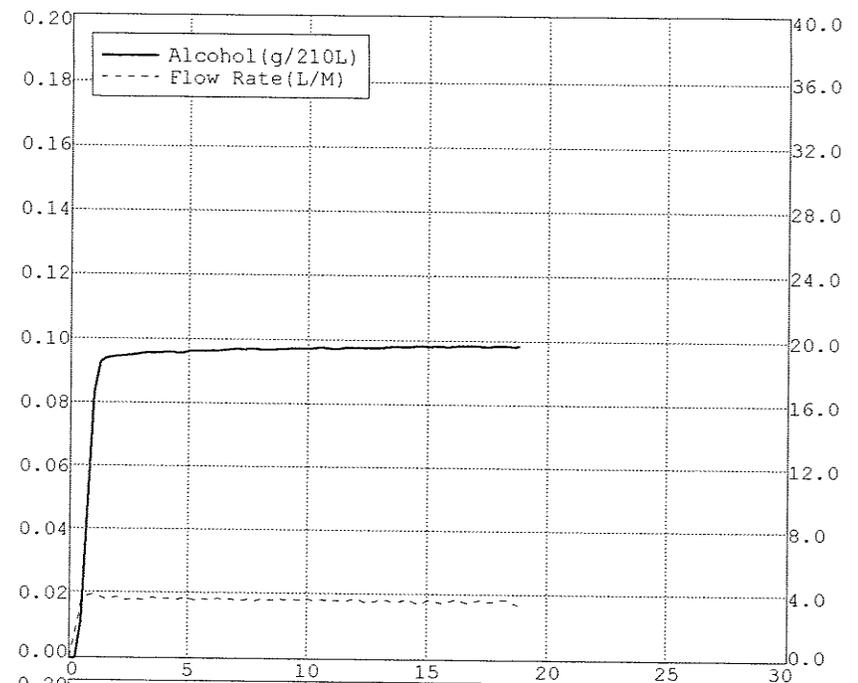

*Charles B Geisler* #24