

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 01/12/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:57
INTERNAL STANDARD	VERIFIED	22:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:57
BLANK TEST	0.00	22:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:58
BLANK TEST	0.00	22:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:00
BLANK TEST	0.00	23:01

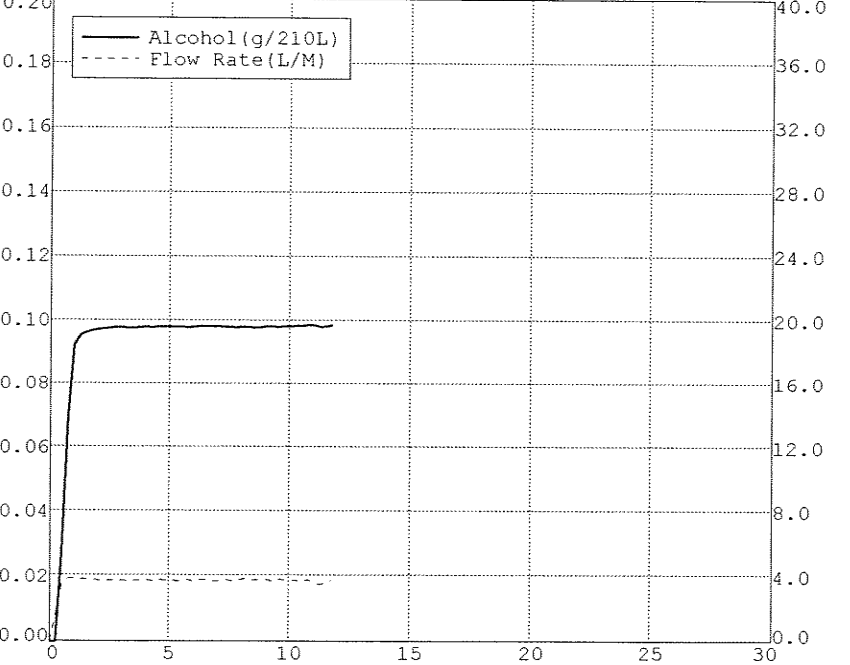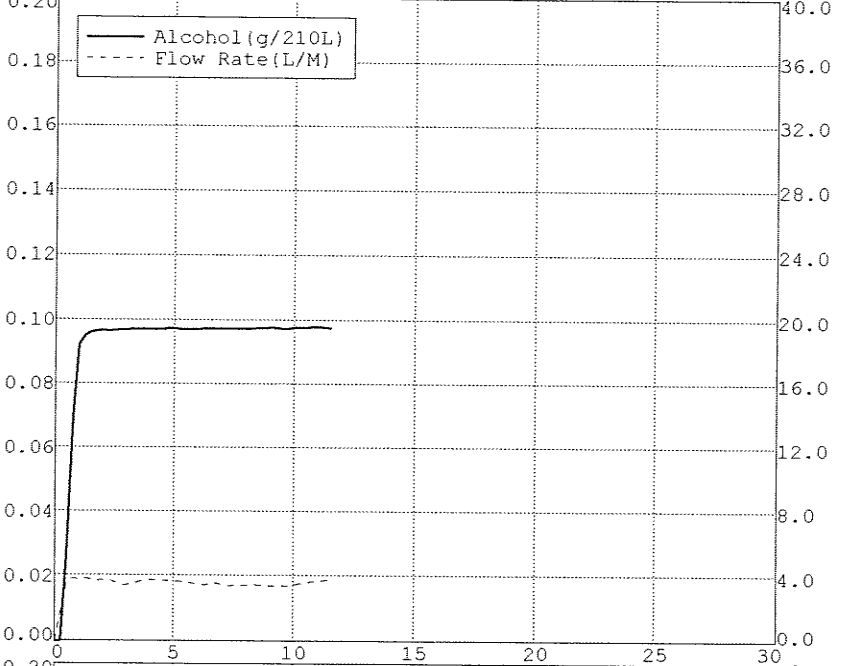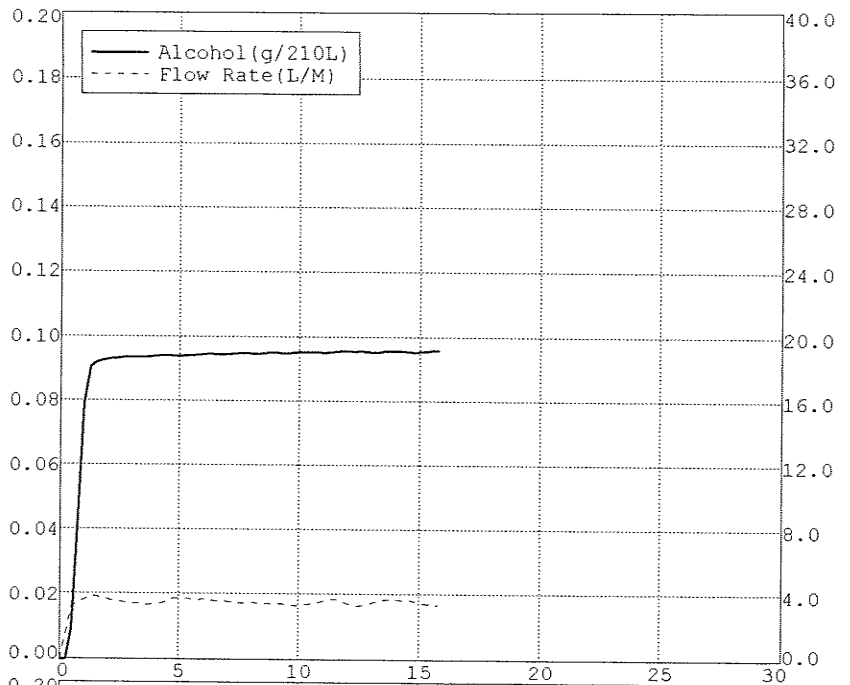

Charles B. Geisler
#2019