

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 01/27/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:44
INTERNAL STANDARD	VERIFIED	22:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:44
BLANK TEST	0.00	22:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:45
BLANK TEST	0.00	22:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:47
BLANK TEST	0.00	22:48

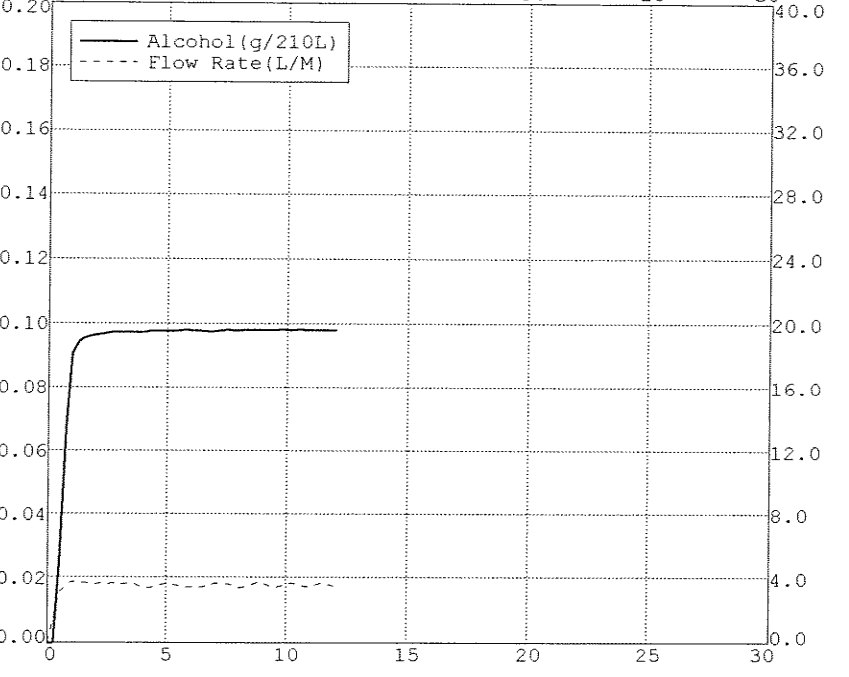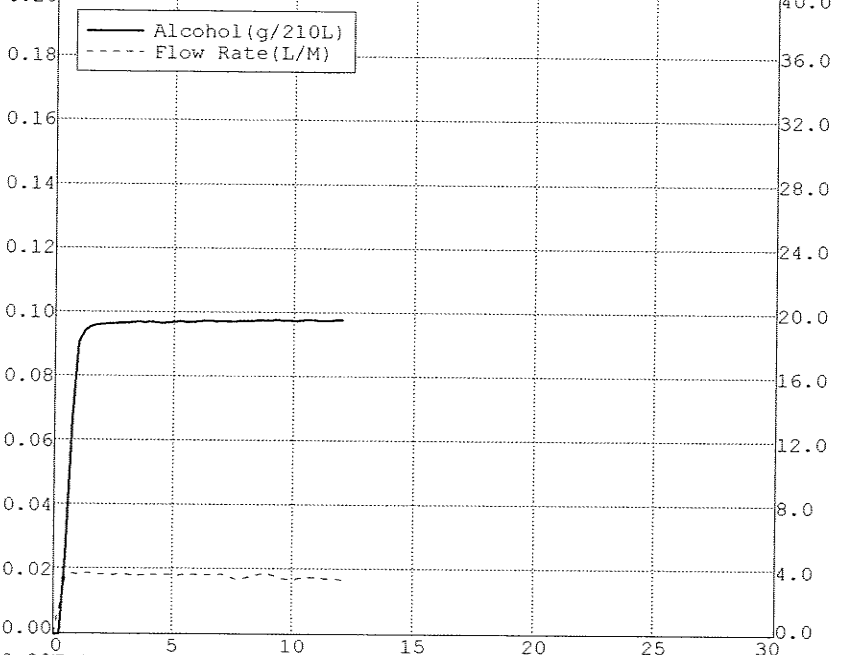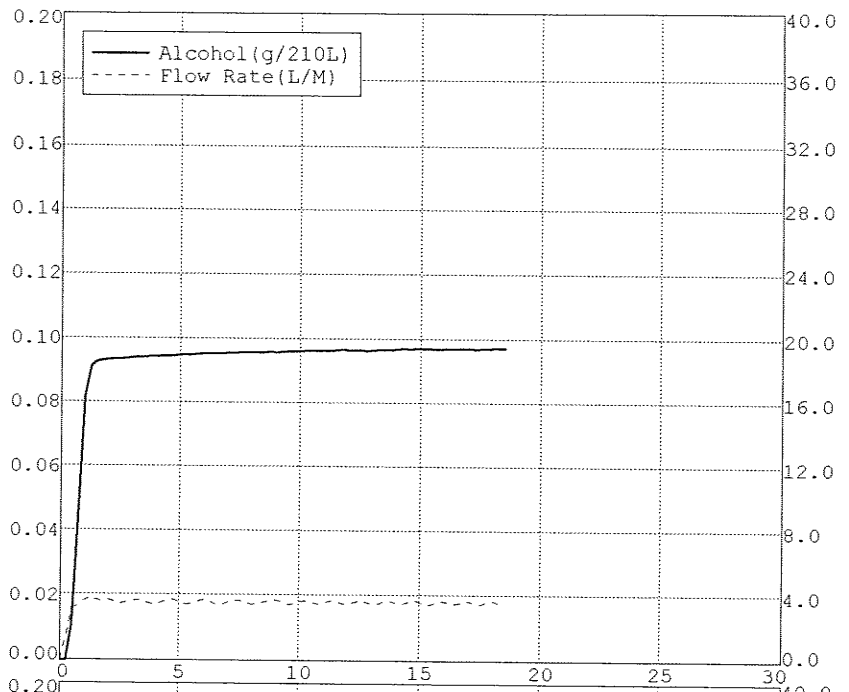

*[Handwritten signatures]*