

SOLUTION CHANGE




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 02/01/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:22
INTERNAL STANDARD	VERIFIED	04:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:23
BLANK TEST	0.00	04:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:24
BLANK TEST	0.00	04:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:25
BLANK TEST	0.00	04:26

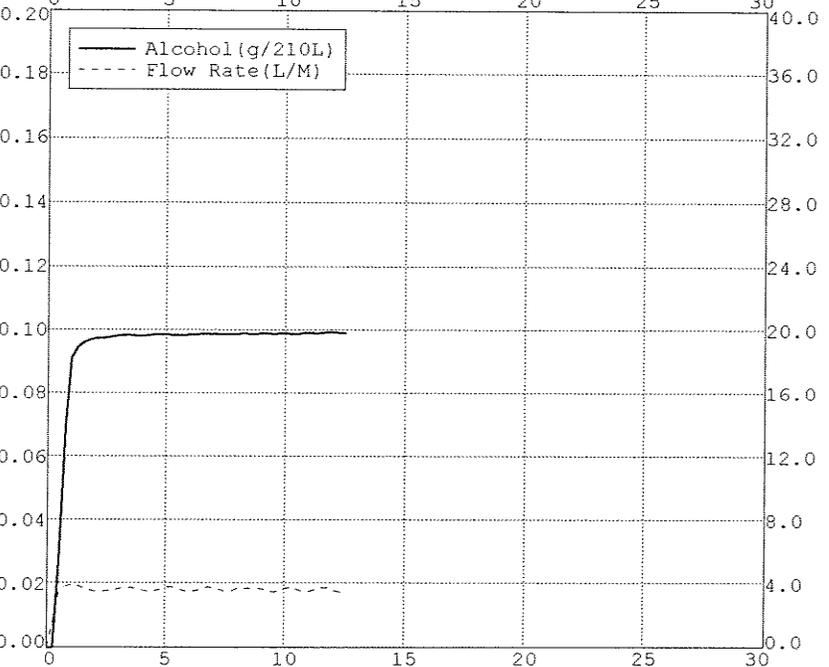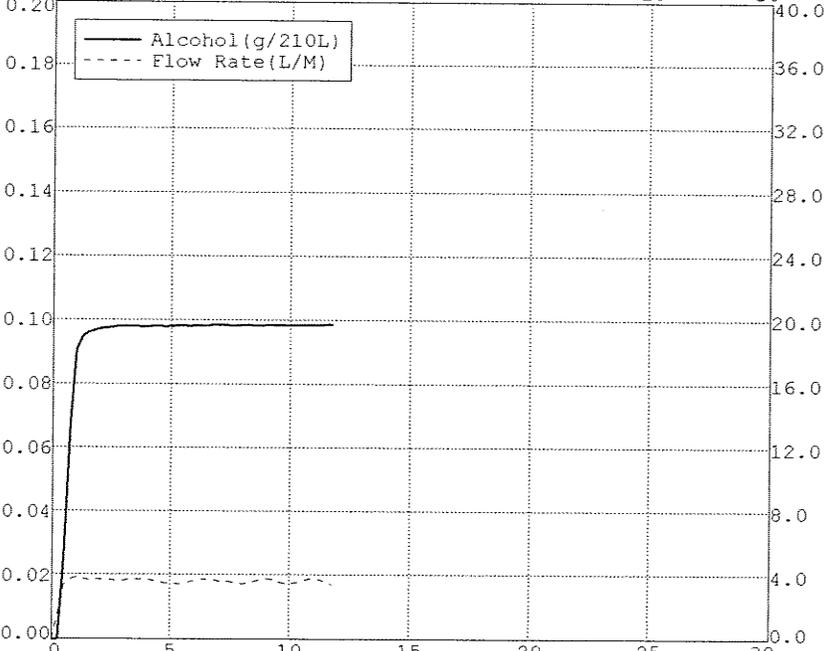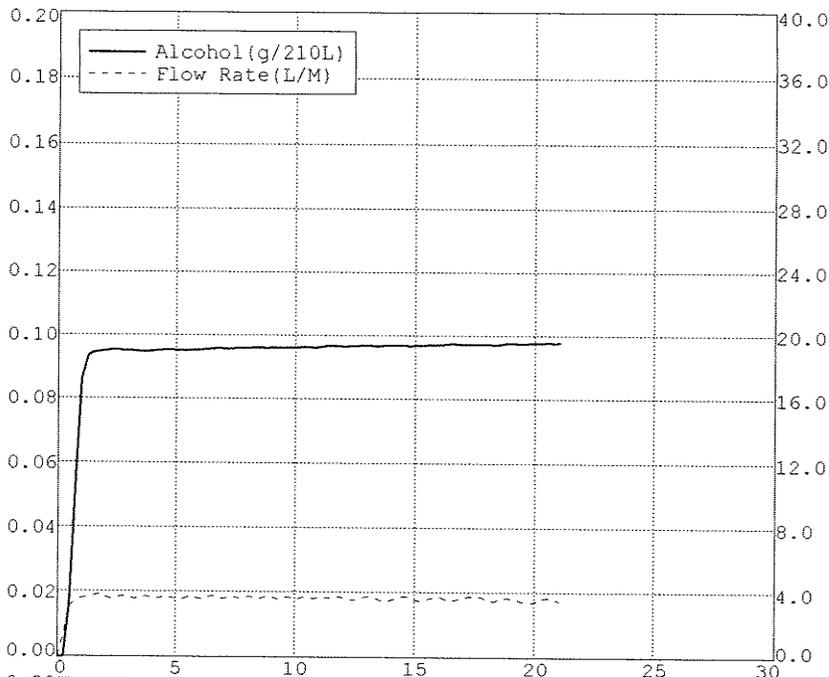

Charles B. Geisler #20