

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 02/05/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:40
INTERNAL STANDARD	VERIFIED	01:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:41
BLANK TEST	0.00	01:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:42
BLANK TEST	0.00	01:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:43
BLANK TEST	0.00	01:44

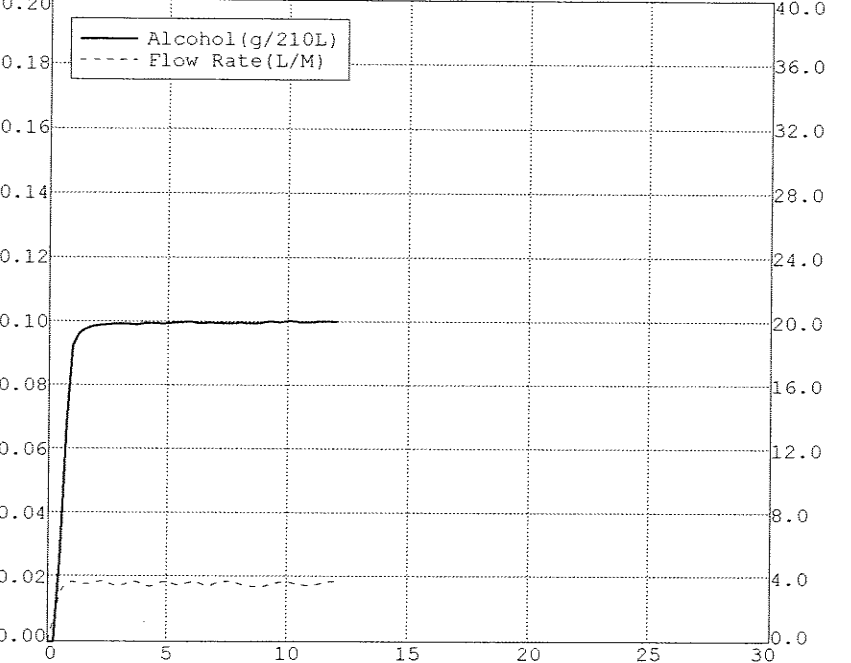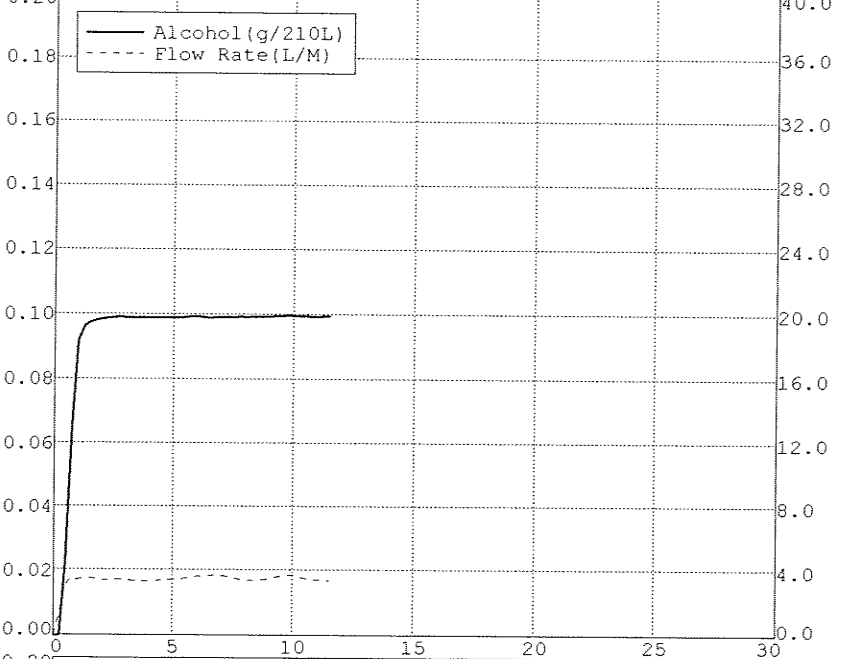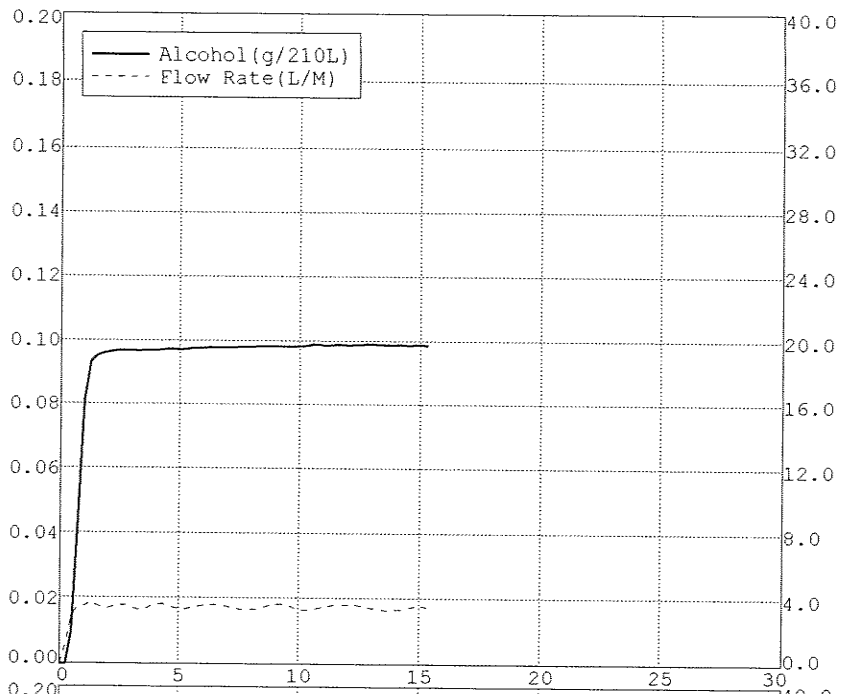

*Sgt. M-B.* *[Signature]* #111