

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 02/10/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:19
INTERNAL STANDARD	VERIFIED	23:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:19
BLANK TEST	0.00	23:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:20
BLANK TEST	0.00	23:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:21
BLANK TEST	0.00	23:22

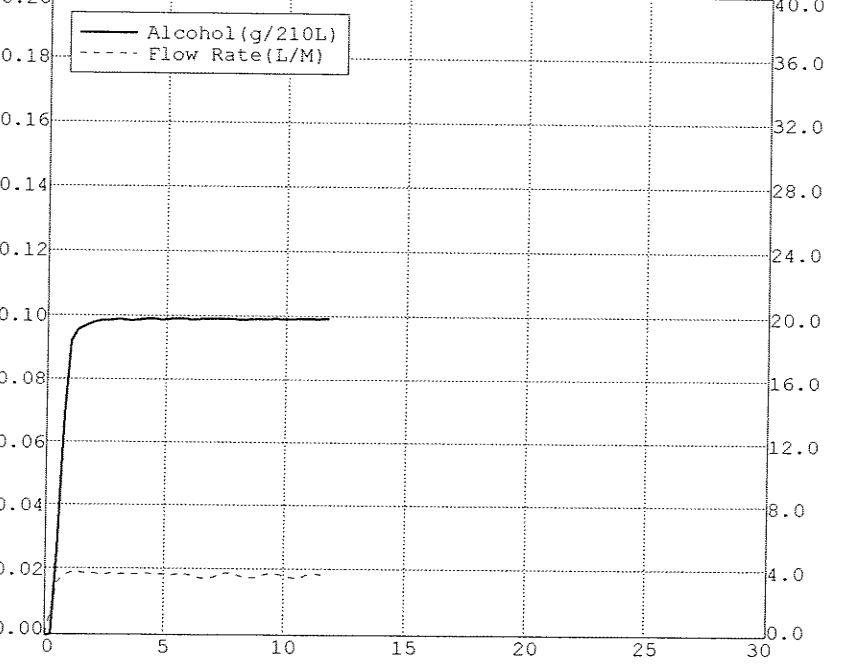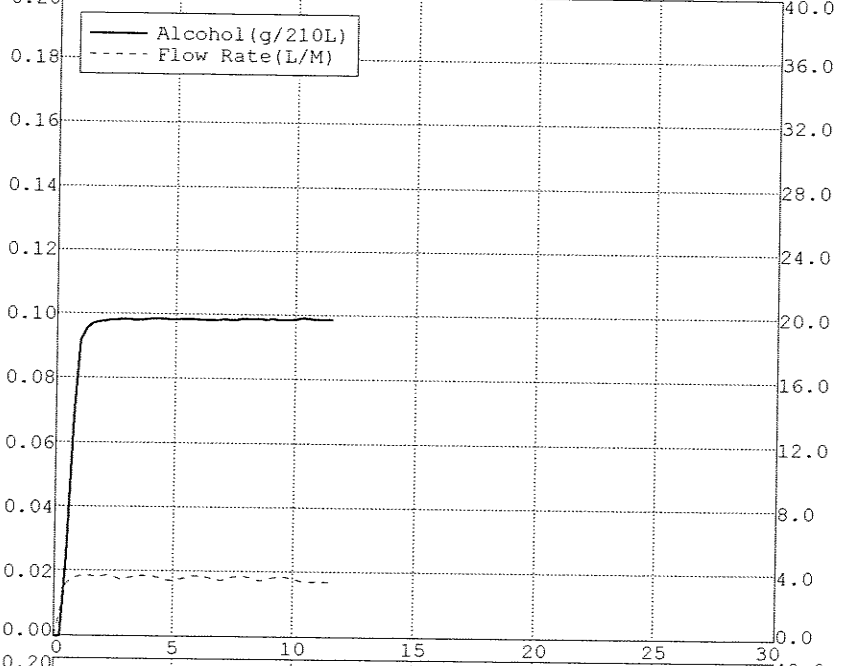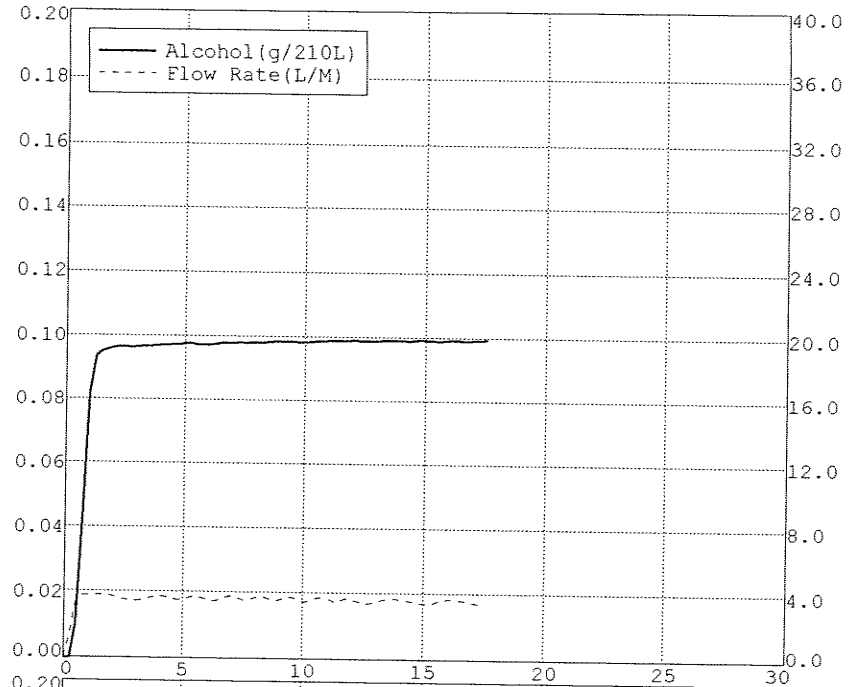

Charles B. Geisler