

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 02/19/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:16
INTERNAL STANDARD	VERIFIED	00:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:17
BLANK TEST	0.00	00:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:18
BLANK TEST	0.00	00:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:19
BLANK TEST	0.00	00:20

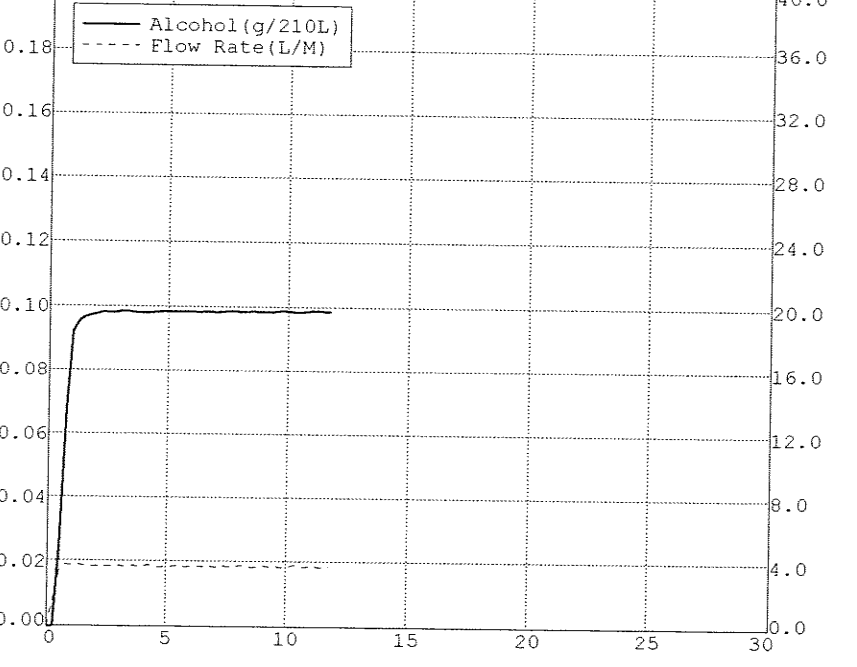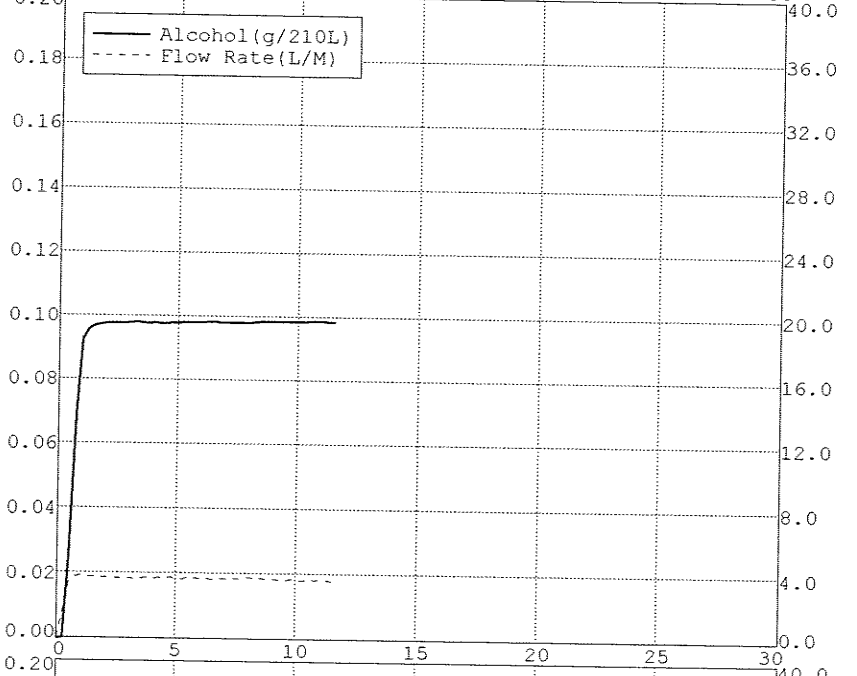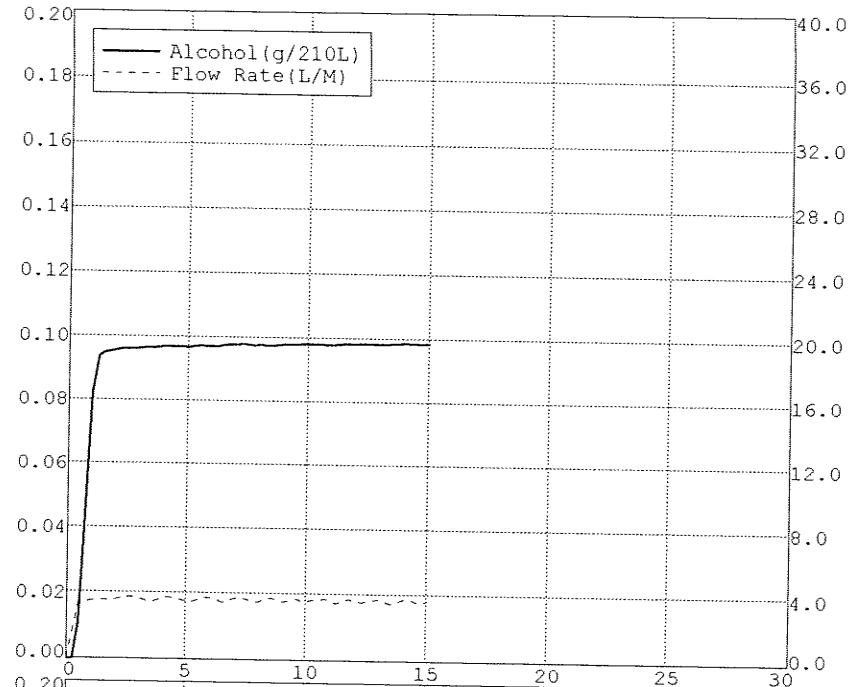

*Charles B. Geisler* #244