

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 02/24/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:33
INTERNAL STANDARD	VERIFIED	23:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:33
BLANK TEST	0.00	23:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:35
BLANK TEST	0.00	23:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:36
BLANK TEST	0.00	23:37

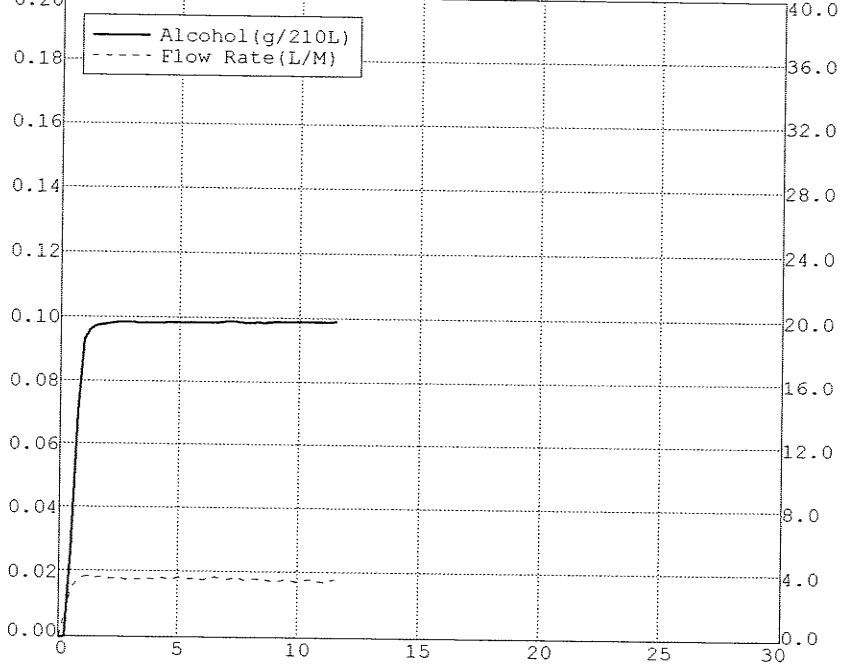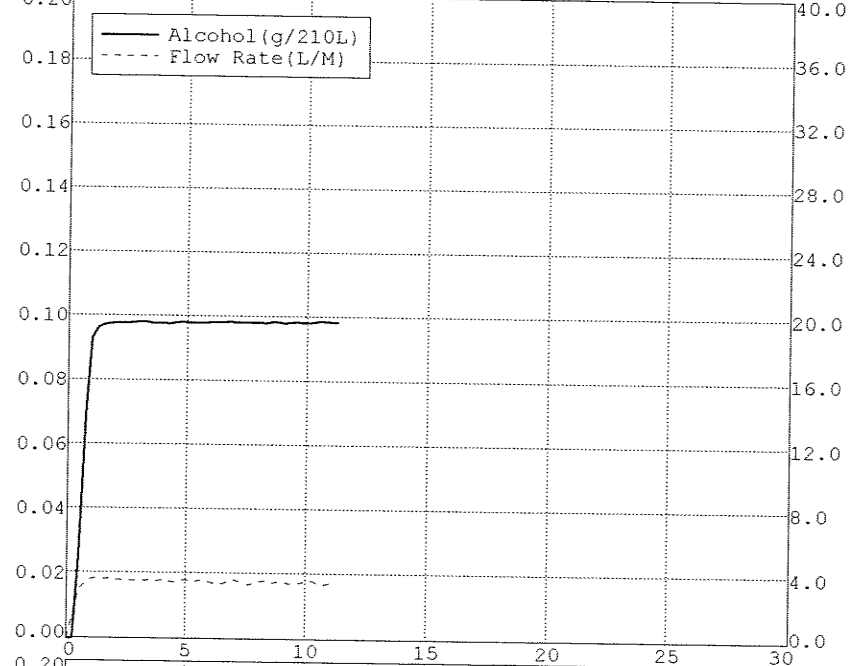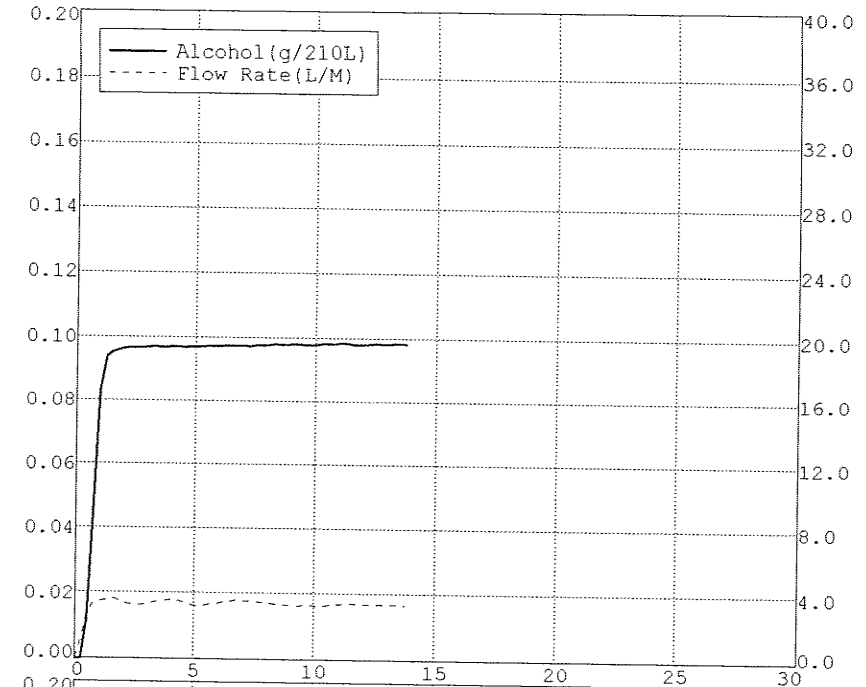

*Charles B. Geisler* #204