

SOLUTION CHANGE




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 03/01/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:40
INTERNAL STANDARD	VERIFIED	00:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:40
BLANK TEST	0.00	00:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:41
BLANK TEST	0.00	00:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:43
BLANK TEST	0.00	00:44

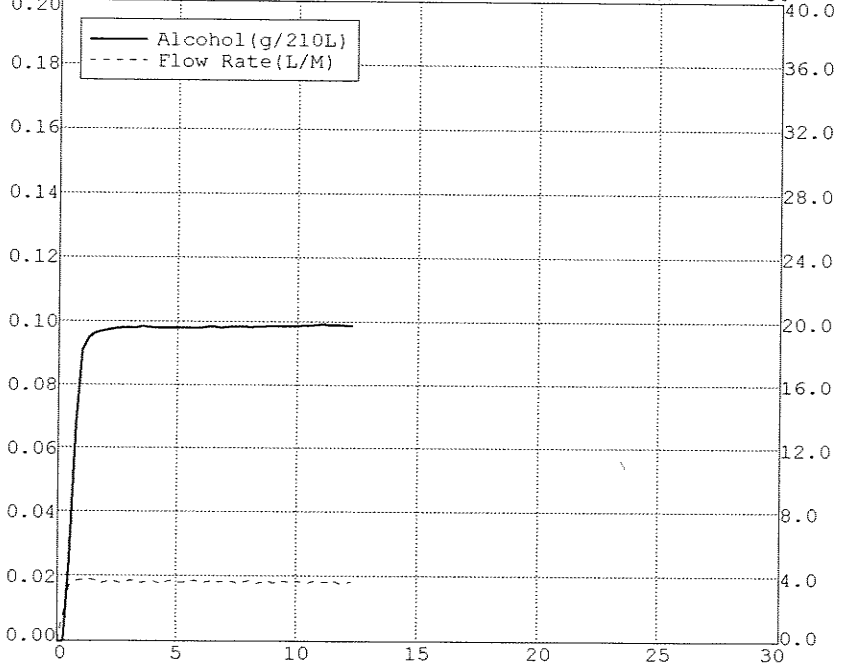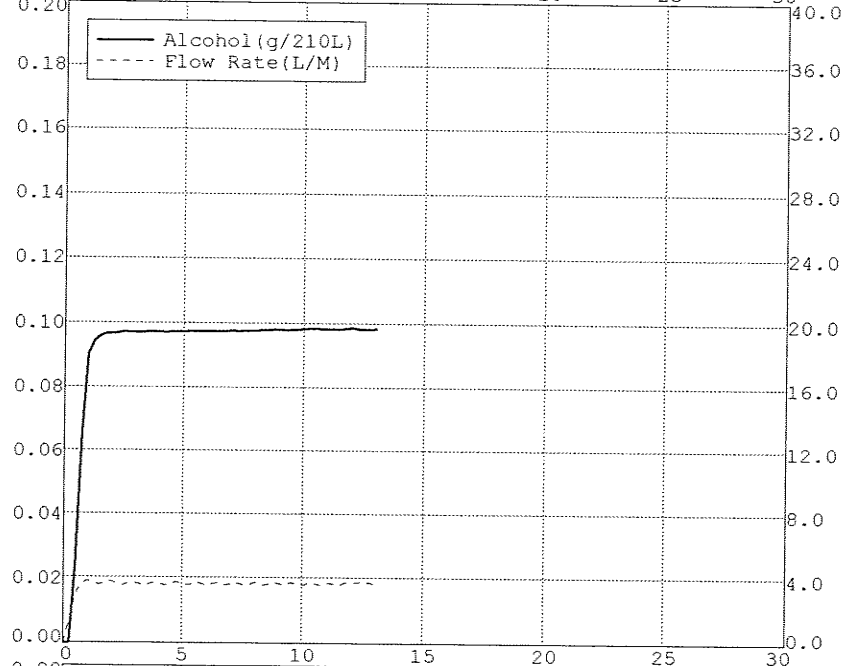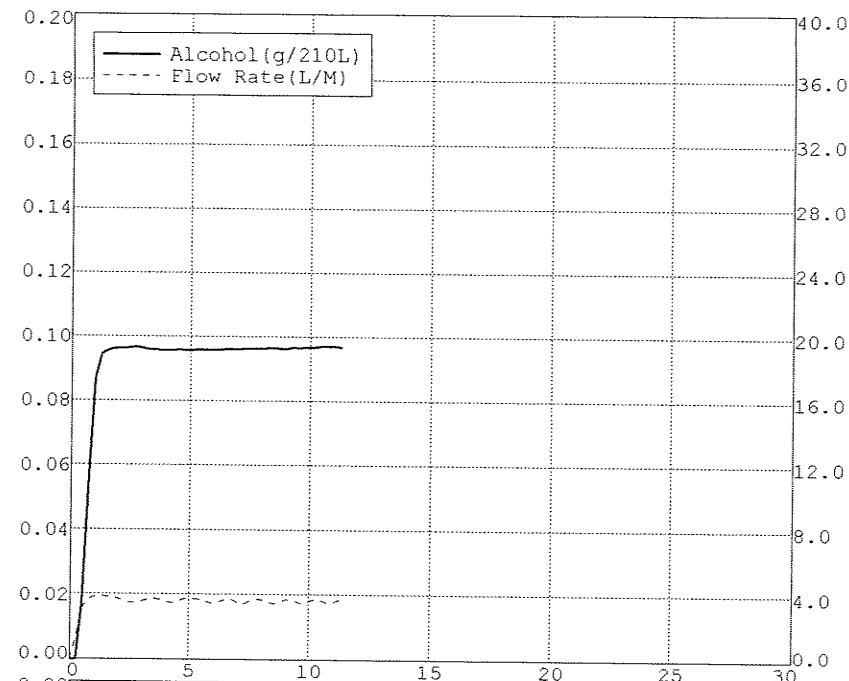

Handwritten signature and initials, likely of Charles B. Geisler, with the number 241 written to the right.