

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 03/09/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:21
INTERNAL STANDARD	VERIFIED	23:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:21
BLANK TEST	0.00	23:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:22
BLANK TEST	0.00	23:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	23:23
BLANK TEST	0.00	23:24

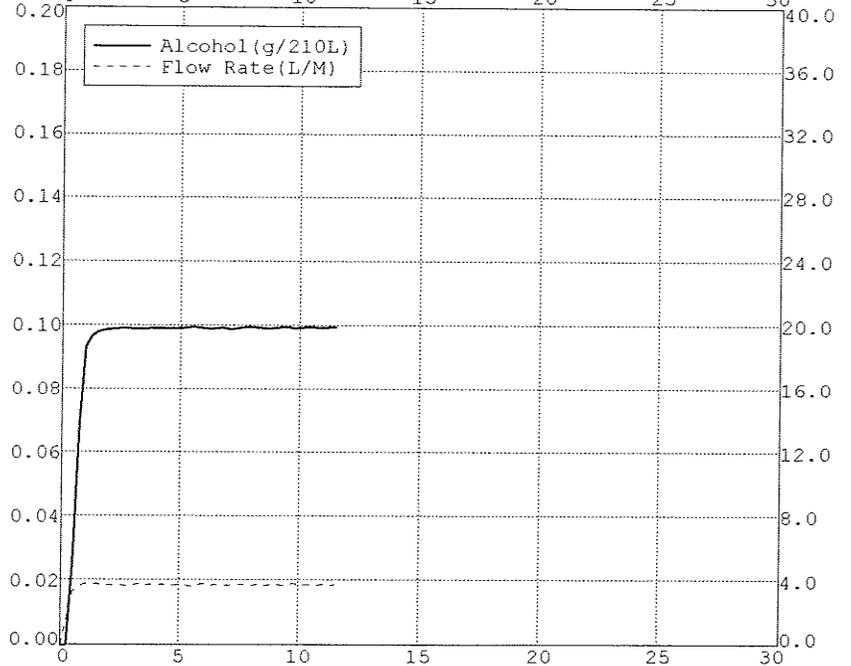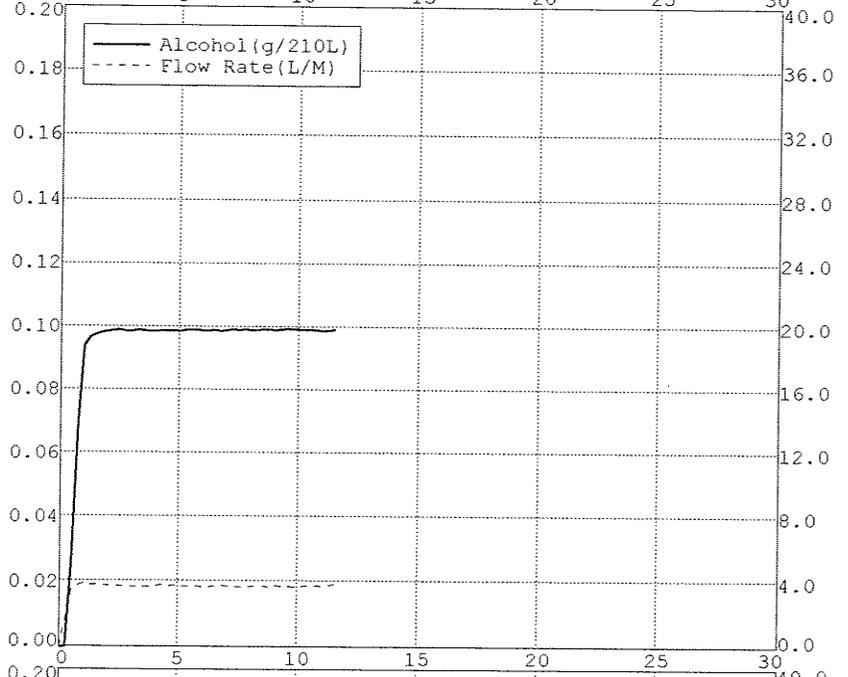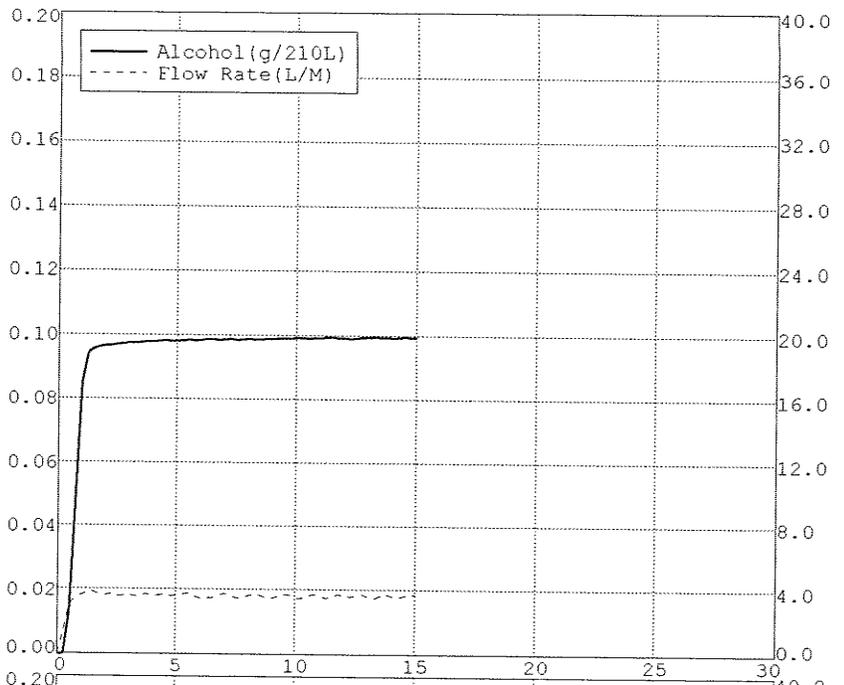

Charles B. Geisler