

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 03/23/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:04
INTERNAL STANDARD	VERIFIED	02:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:04
BLANK TEST	0.00	02:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:05
BLANK TEST	0.00	02:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:07
BLANK TEST	0.00	02:08

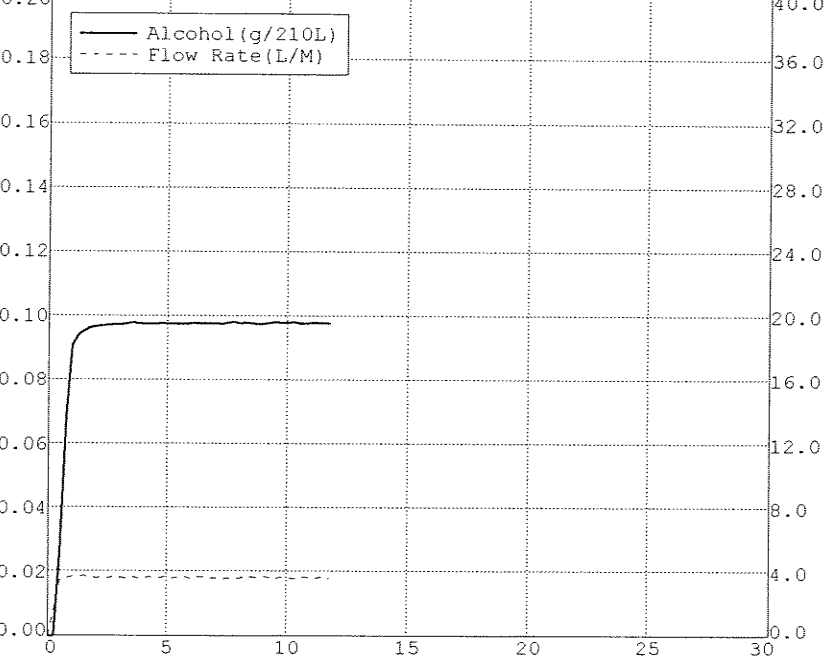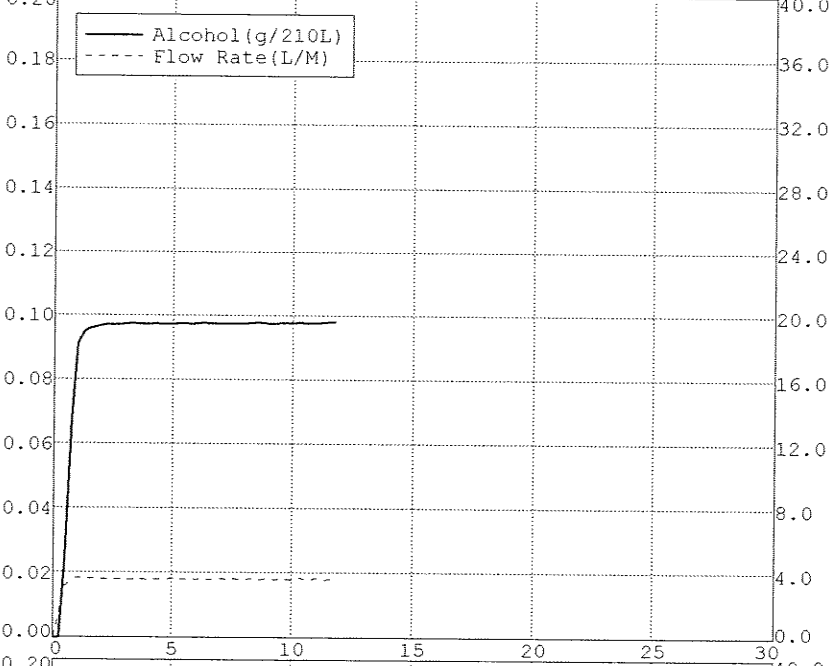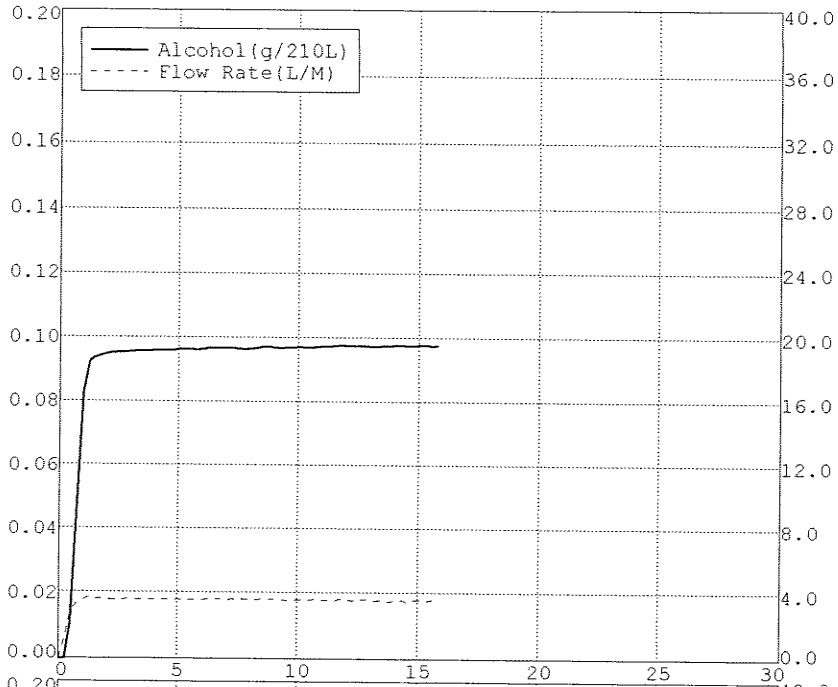

*Signature: Charles B. Geisler*