

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 04/24/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:32
INTERNAL STANDARD	VERIFIED	23:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:33
BLANK TEST	0.00	23:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:34
BLANK TEST	0.00	23:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:35
BLANK TEST	0.00	23:36

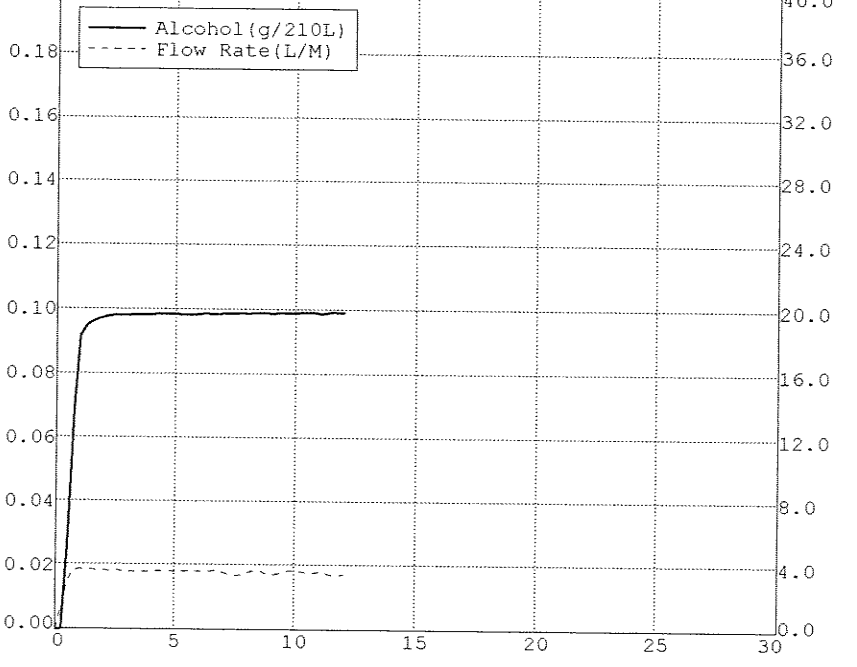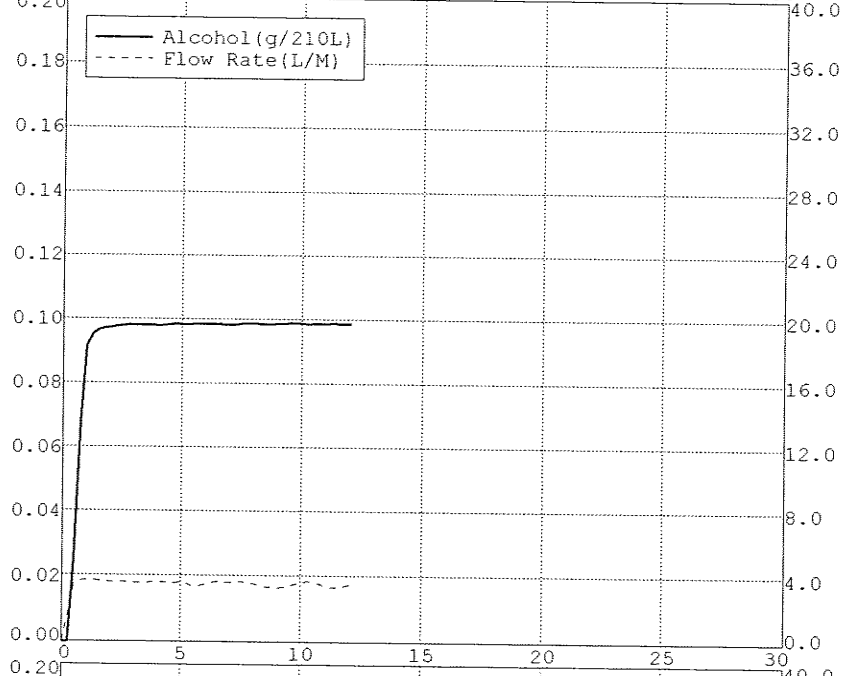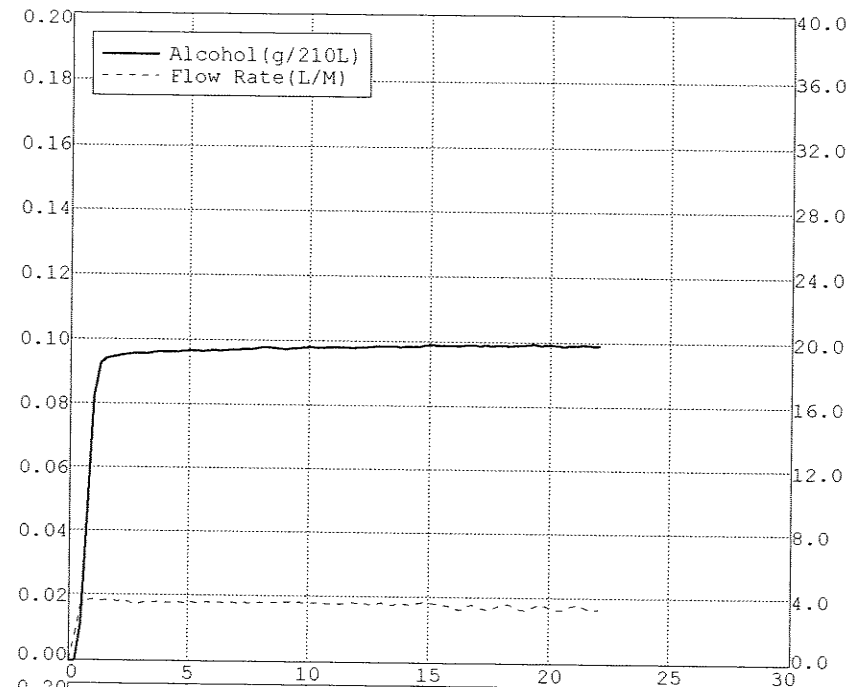

Handwritten signature: Charles B. Geisler