

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 05/15/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:30
INTERNAL STANDARD	VERIFIED	00:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:31
BLANK TEST	0.00	00:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:32
BLANK TEST	0.00	00:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:33
BLANK TEST	0.00	00:34

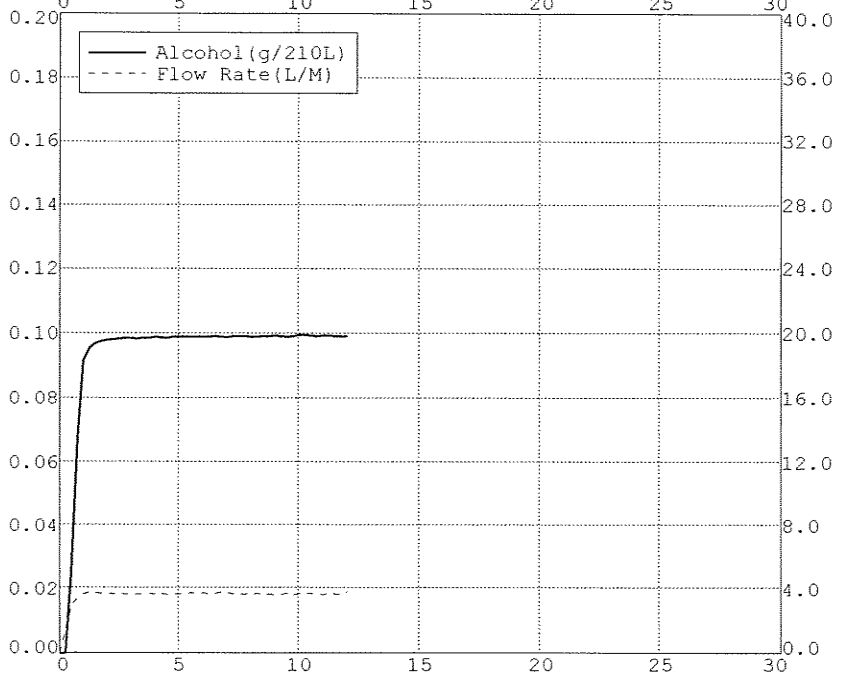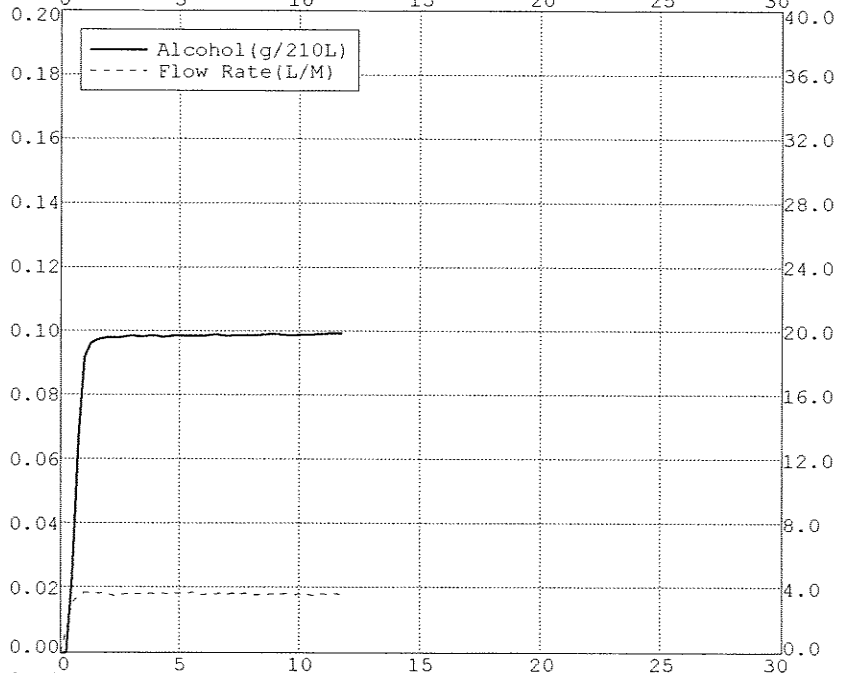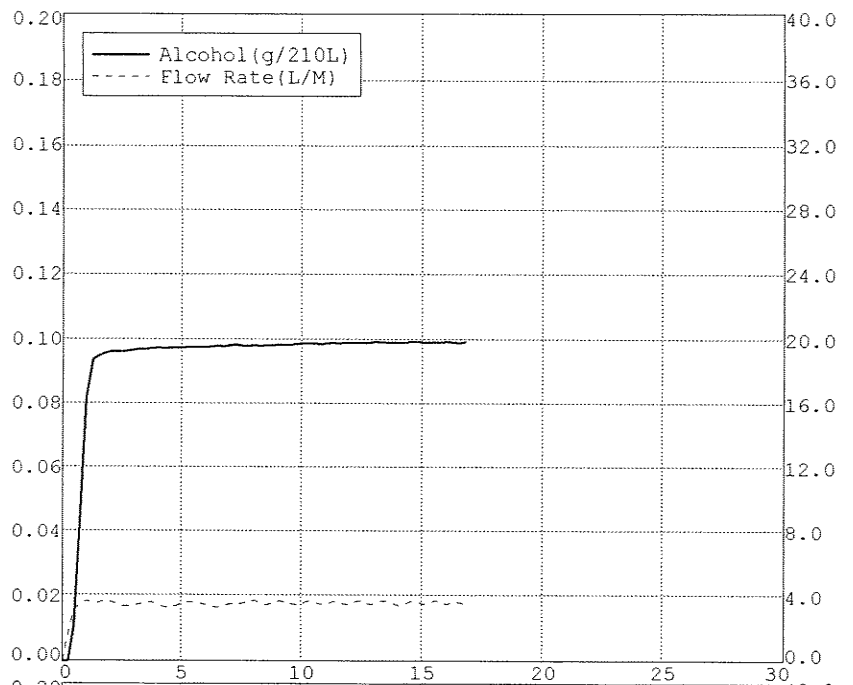

[Handwritten signature]
#2W