

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 05/29/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:14
INTERNAL STANDARD	VERIFIED	01:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:15
BLANK TEST	0.00	01:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:16
BLANK TEST	0.00	01:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:17
BLANK TEST	0.00	01:18

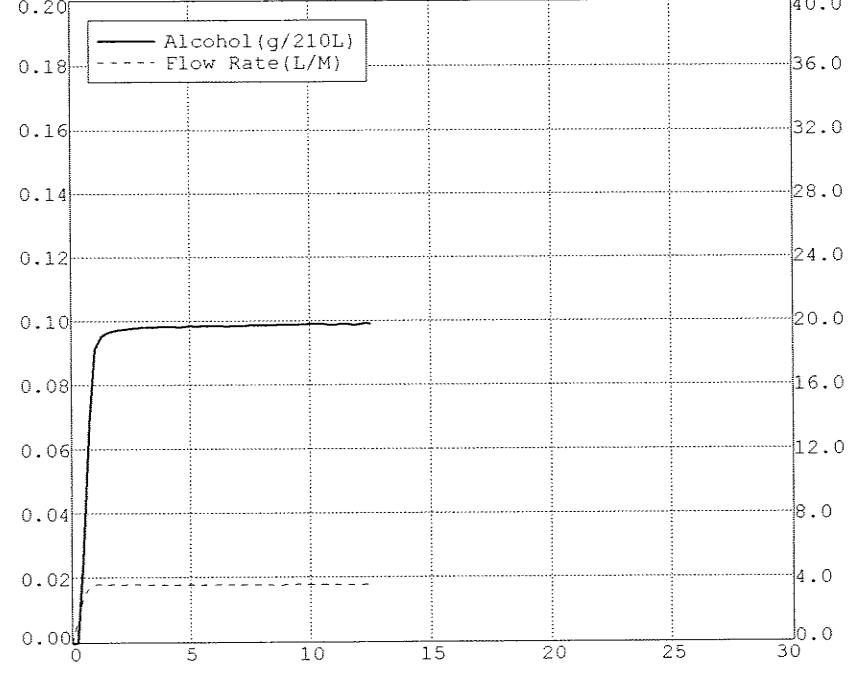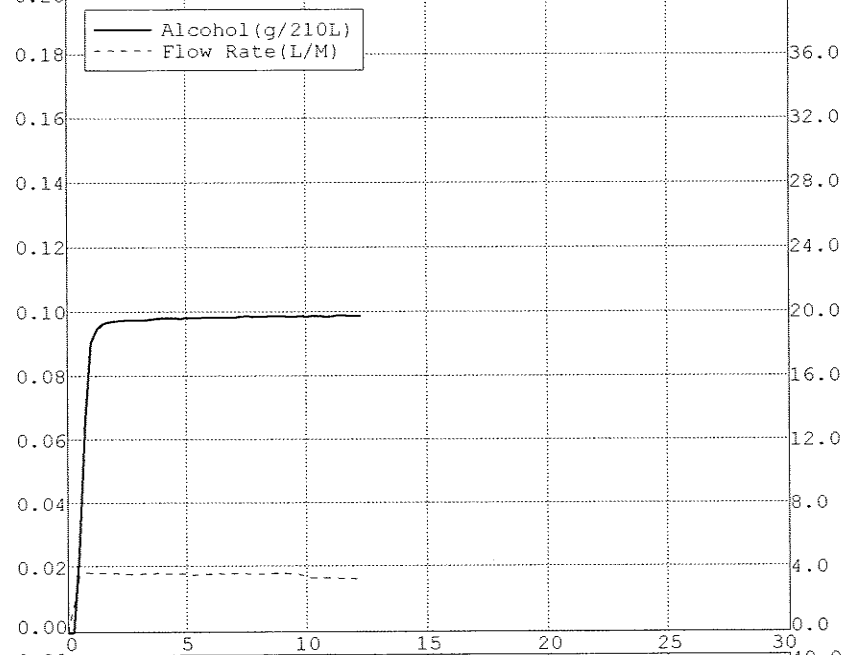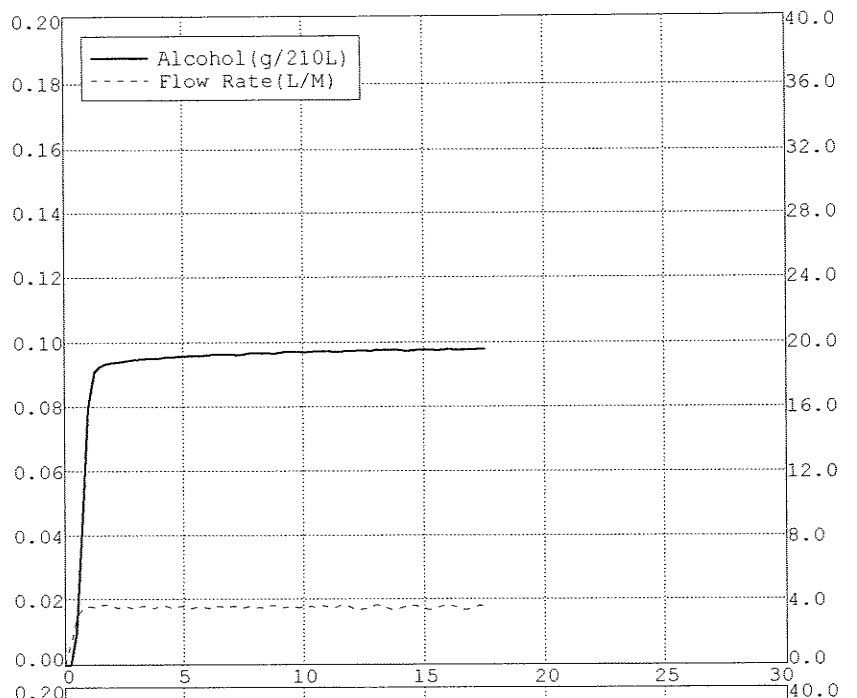

Charles B. Geisler