

SOLUTION CHANGE




WARREN COUNTY
 SHERIFF'S OFFICE
 DATAMASTER dmt: 144506

Date: 06/01/2019

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:49
INTERNAL STANDARD	VERIFIED	23:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:49
BLANK TEST	0.00	23:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:50
BLANK TEST	0.00	23:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:52
BLANK TEST	0.00	23:52

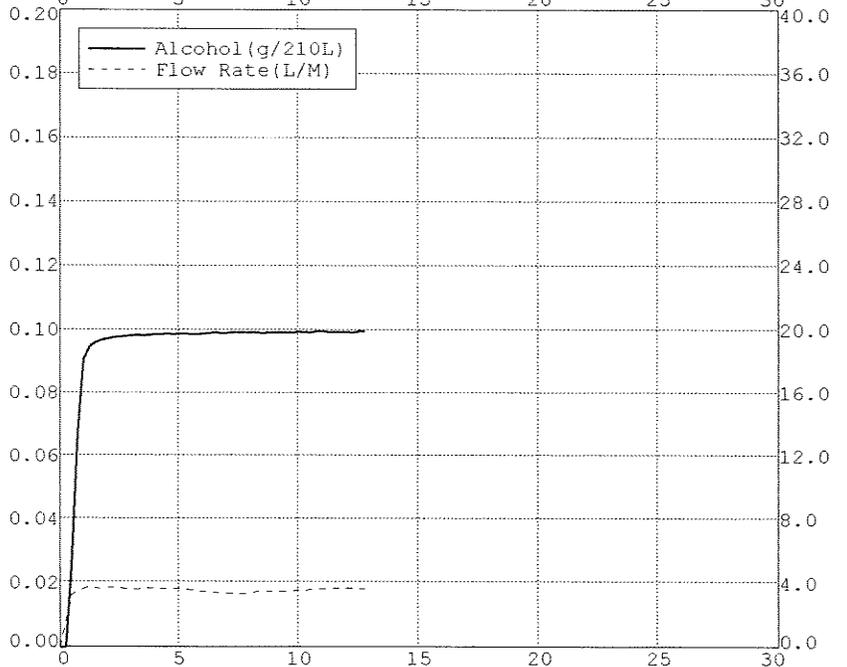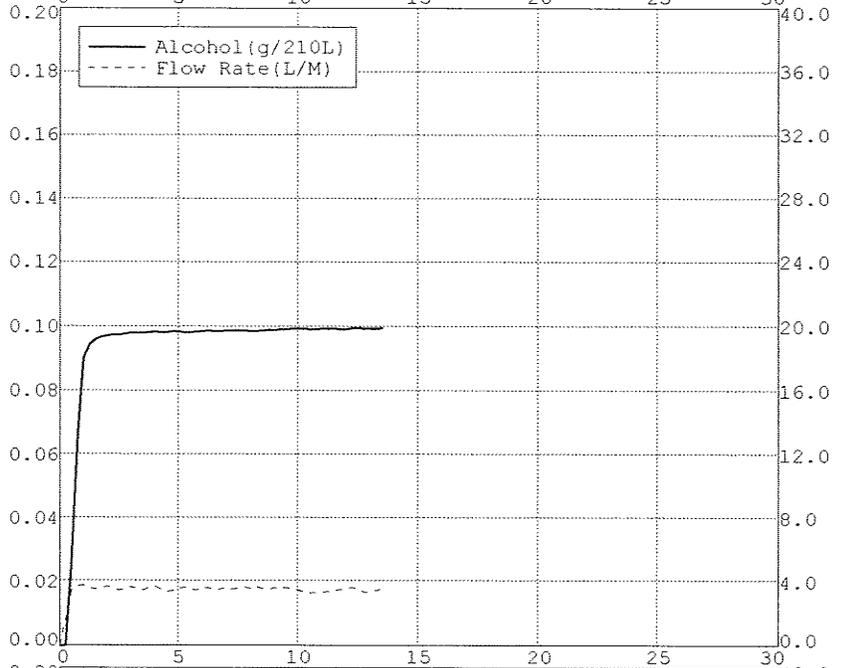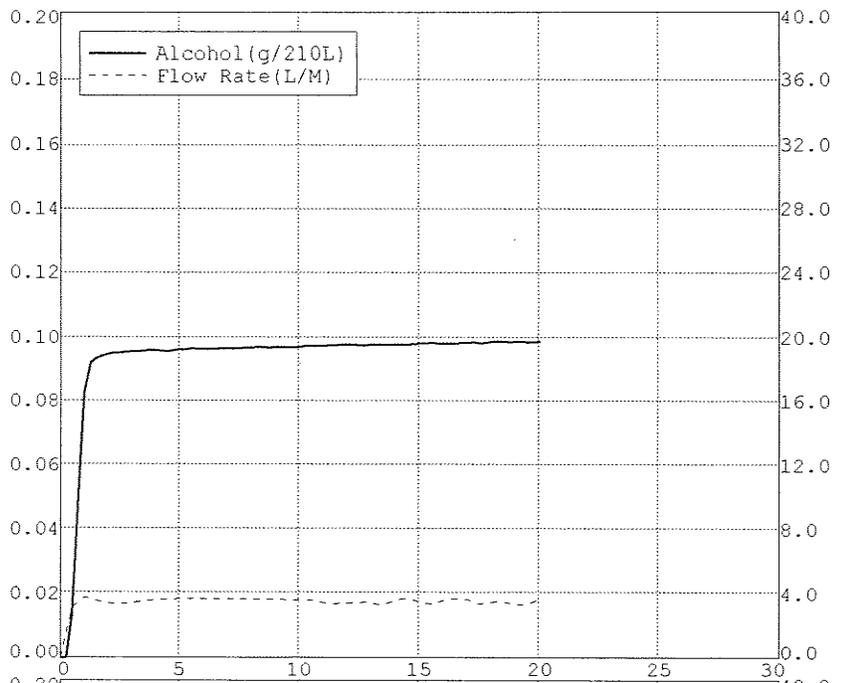

Charles B. Geisler
 C.B.G. #20