

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 06/24/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:41
INTERNAL STANDARD	VERIFIED	13:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:42
BLANK TEST	0.00	13:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:43
BLANK TEST	0.00	13:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:44
BLANK TEST	0.00	13:45

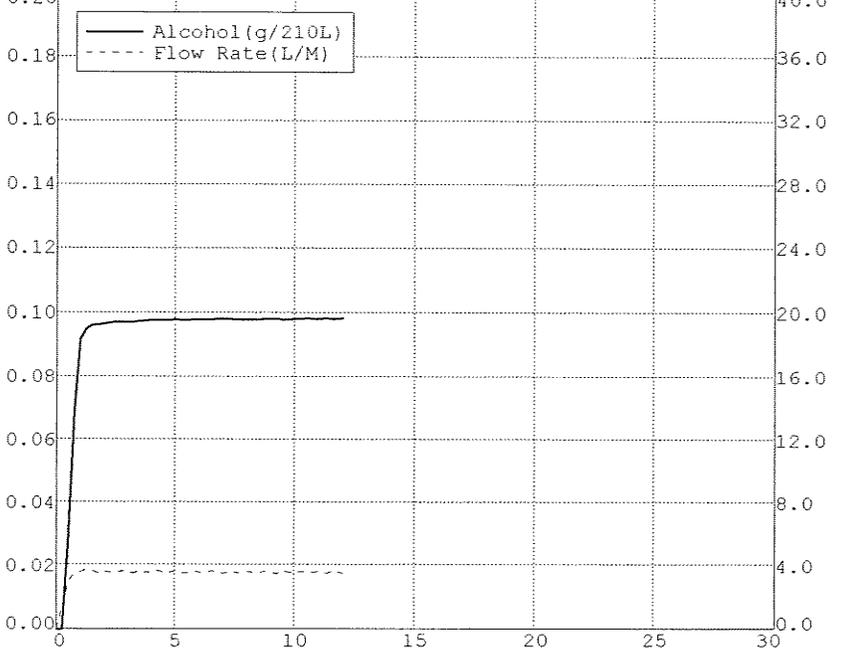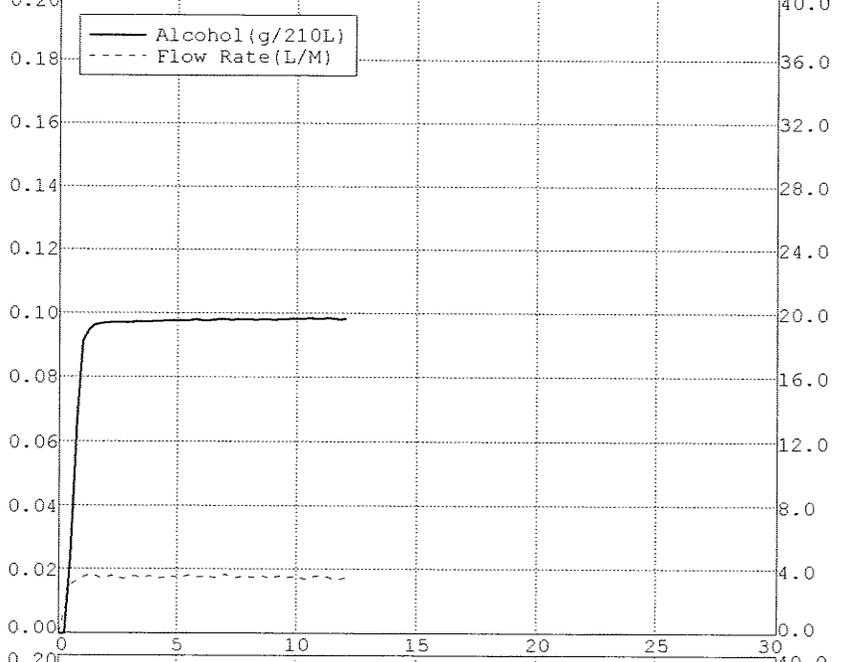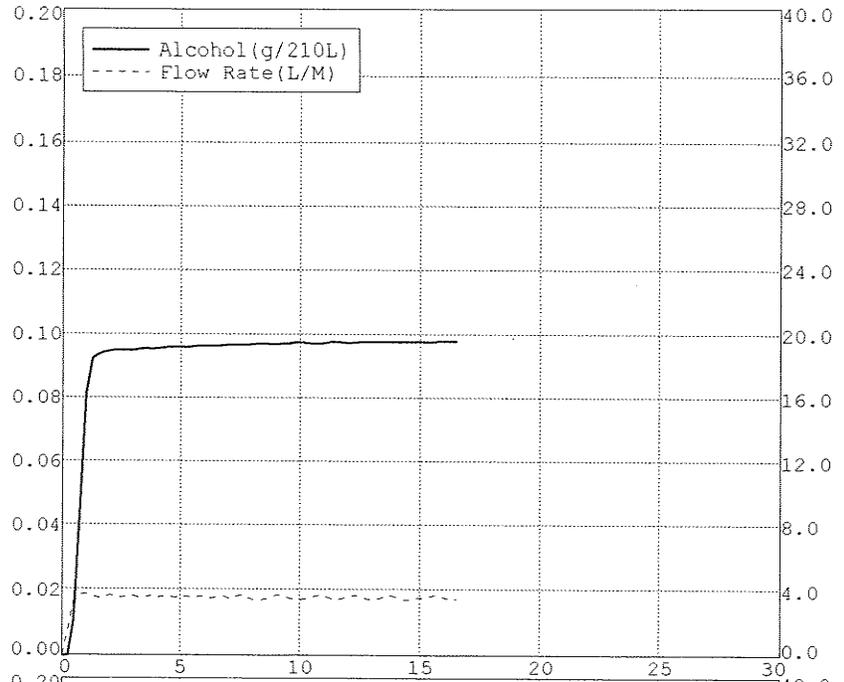

*Charles B. Geisler* #244