

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 07/22/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:55
INTERNAL STANDARD	VERIFIED	23:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:56
BLANK TEST	0.00	23:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:57
BLANK TEST	0.00	23:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:58
BLANK TEST	0.00	23:59

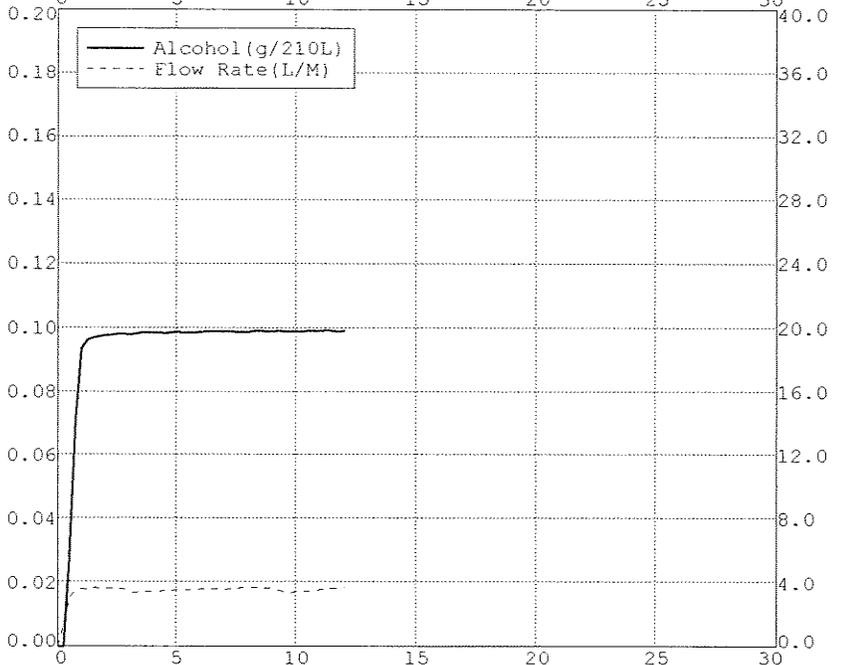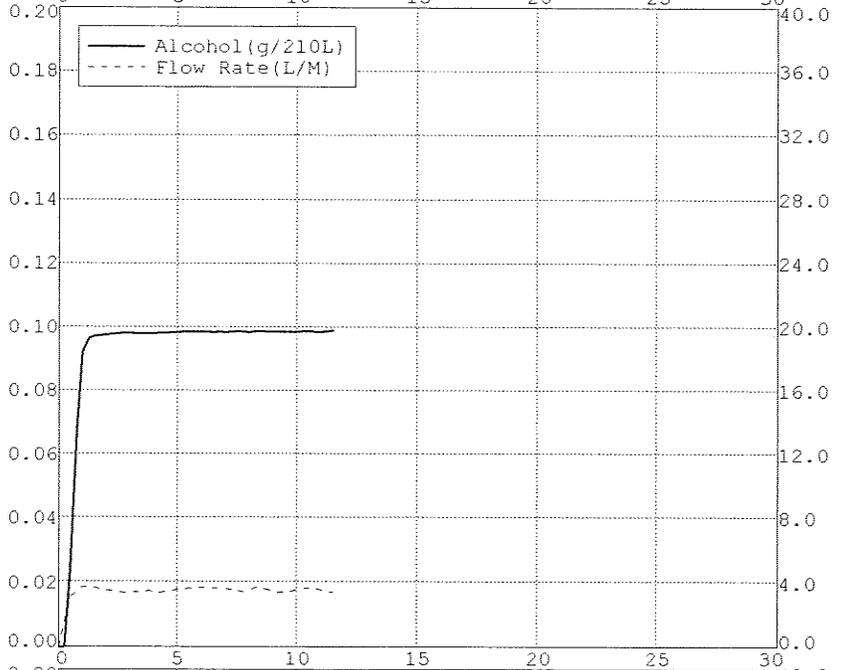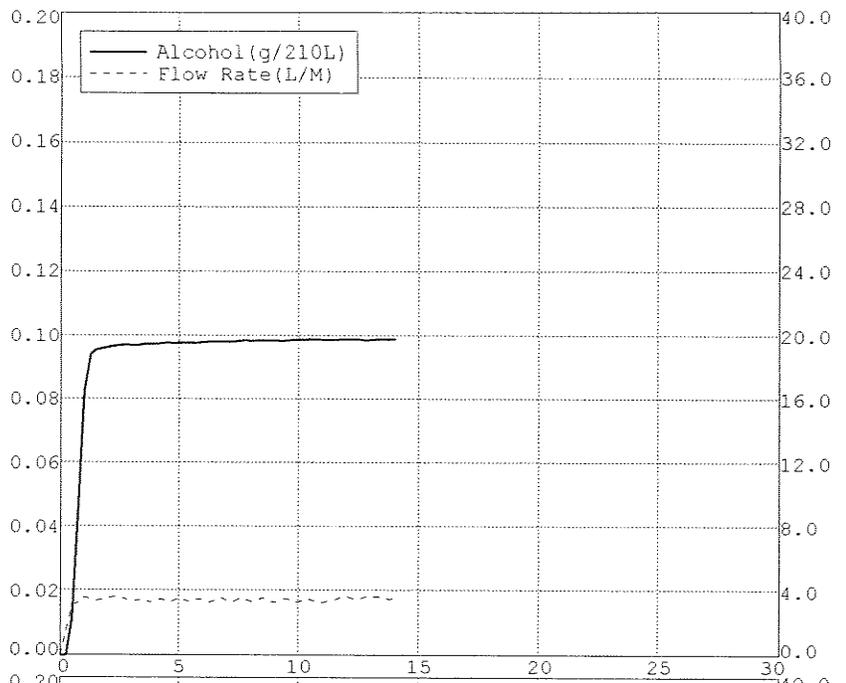

[Handwritten signatures and initials]
#2W