

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 07/29/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:51
INTERNAL STANDARD	VERIFIED	00:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:52
BLANK TEST	0.00	00:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:53
BLANK TEST	0.00	00:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:54
BLANK TEST	0.00	00:55

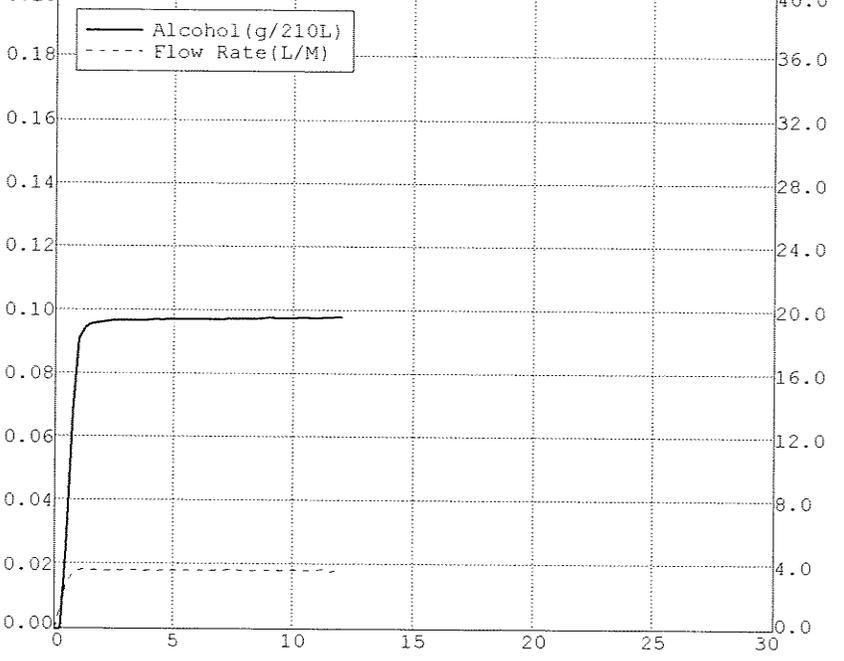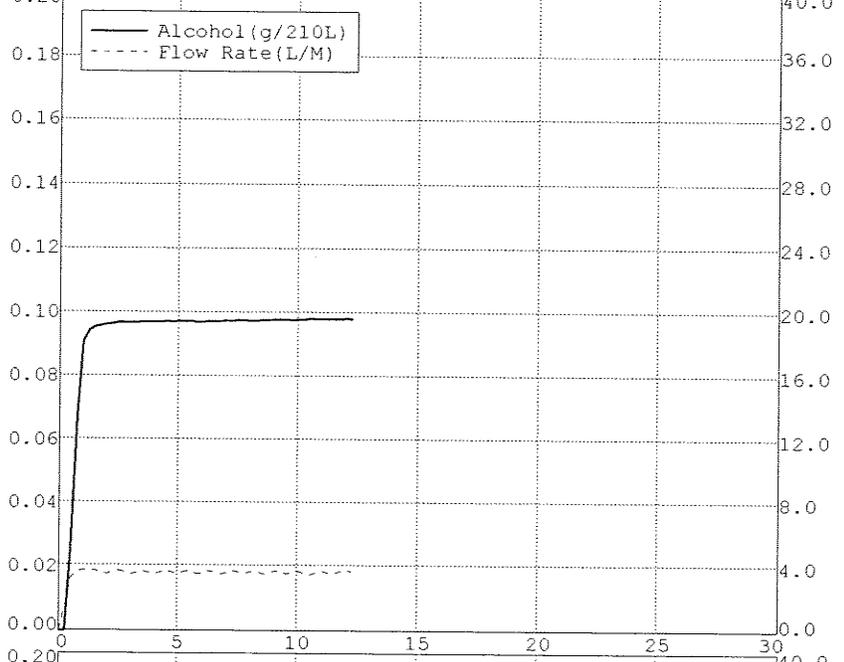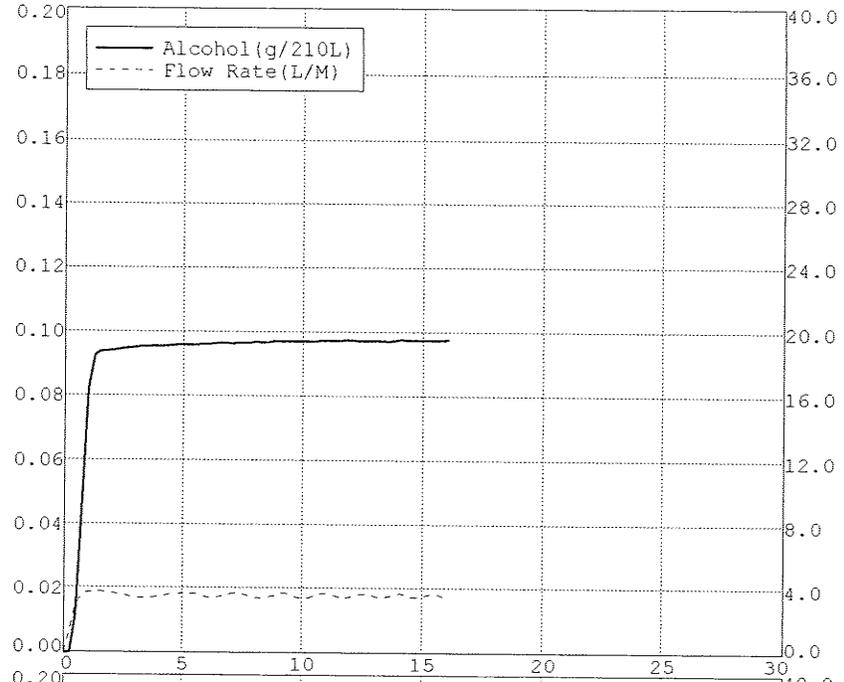

Sgt. C. B. Geisler