

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 08/09/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:11
INTERNAL STANDARD	VERIFIED	23:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:11
BLANK TEST	0.00	23:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:12
BLANK TEST	0.00	23:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:13
BLANK TEST	0.00	23:14

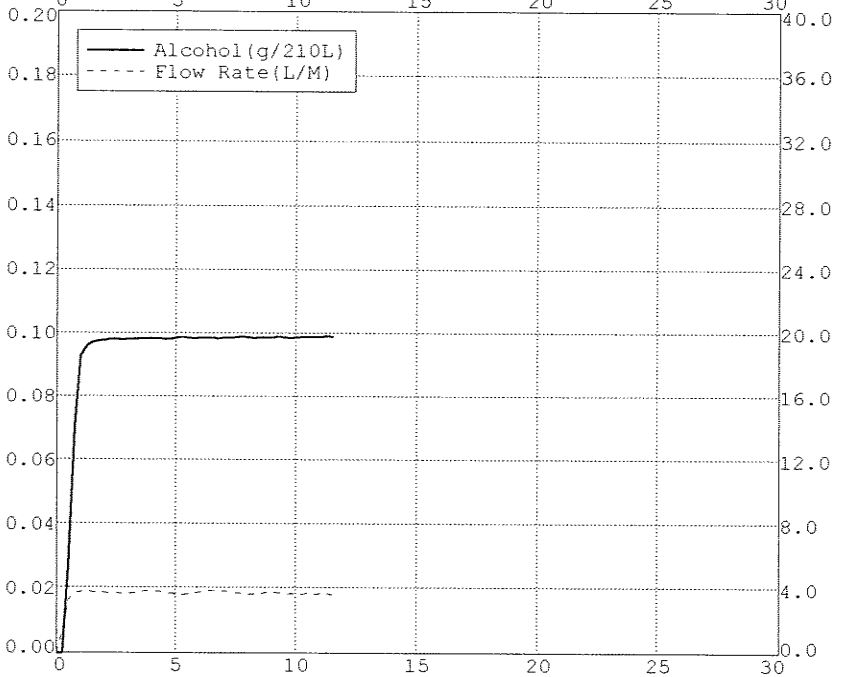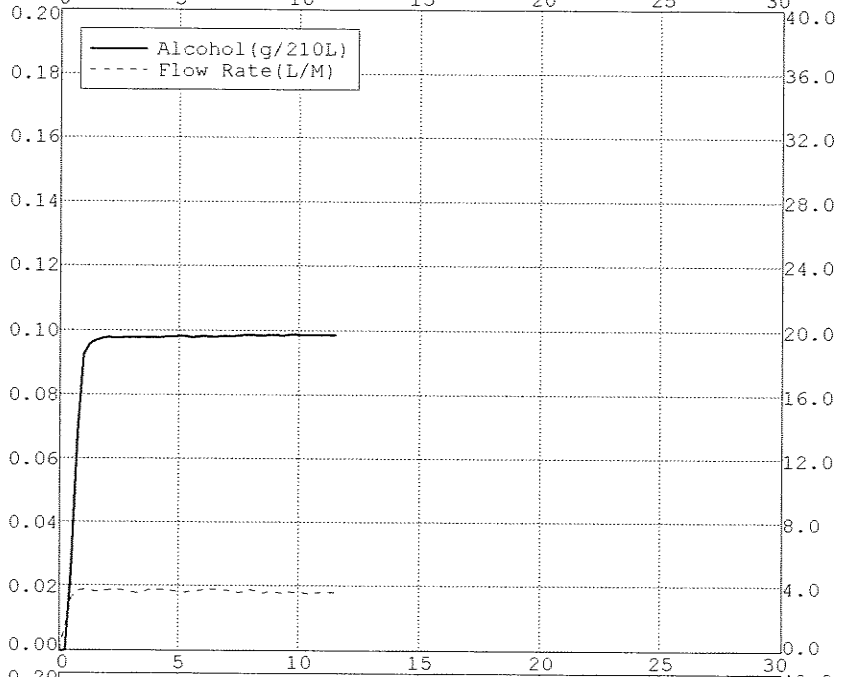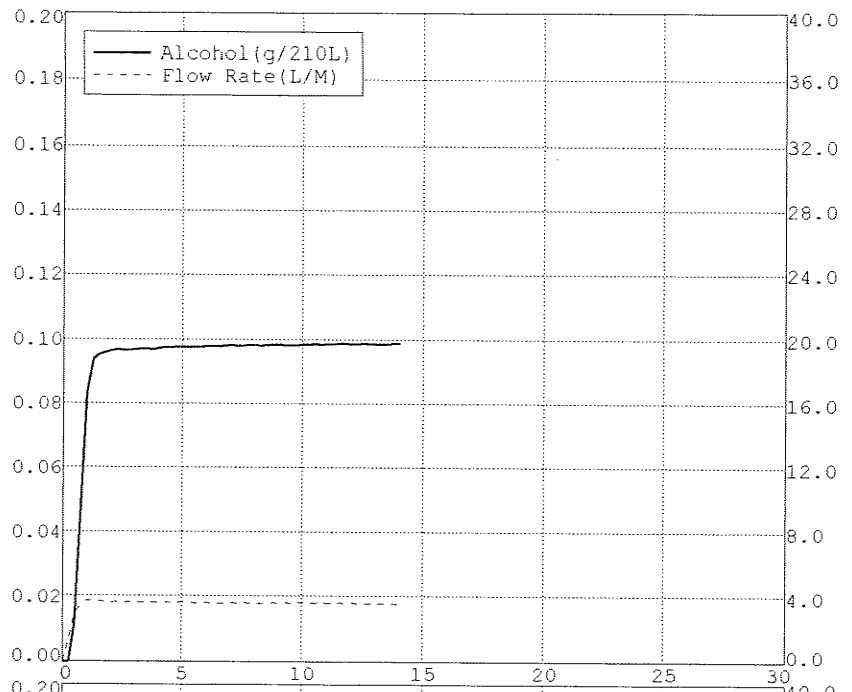

Handwritten signature: C. B. Geisler