

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 08/15/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19130

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 05:03 |
| INTERNAL STANDARD       | VERIFIED | 05:03 |
| REFERENCE STANDARD TEMP | 34.00c   |       |
| REFERENCE STANDARD      | 0.09     | 05:03 |
| BLANK TEST              | 0.00     | 05:04 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.09     | 05:05 |
| BLANK TEST              | 0.00     | 05:05 |
| REFERENCE STANDARD TEMP | 34.00c   |       |
| REFERENCE STANDARD      | 0.09     | 05:06 |
| BLANK TEST              | 0.00     | 05:07 |

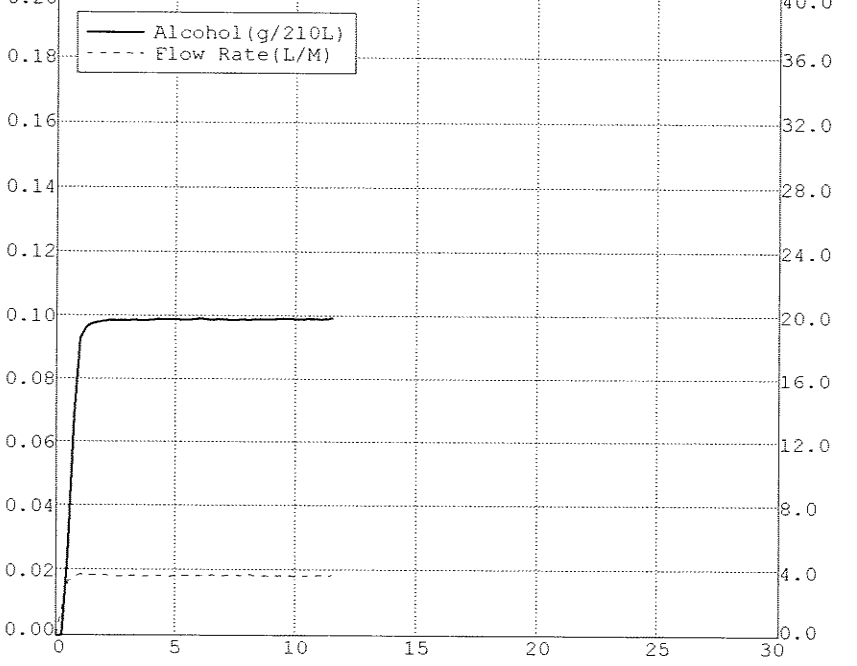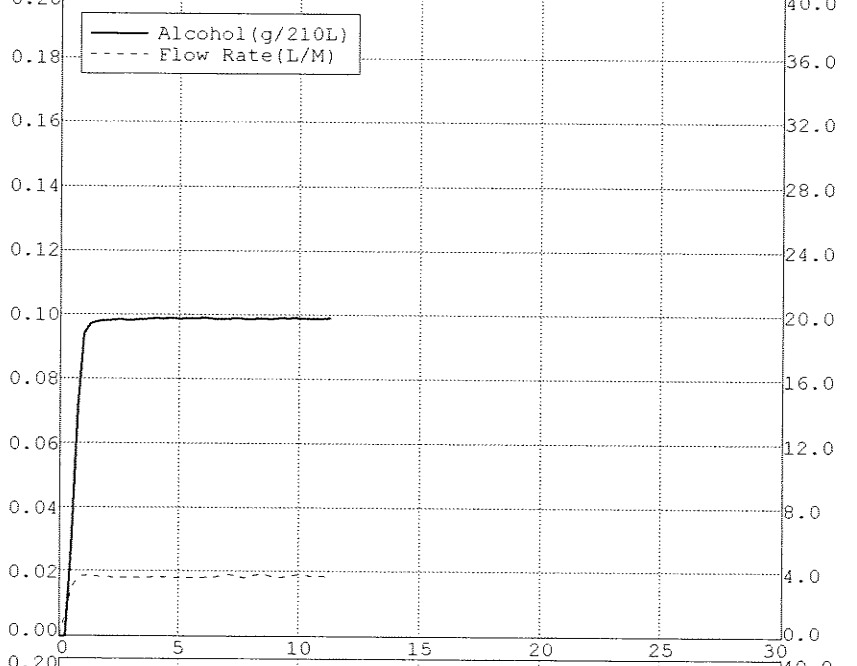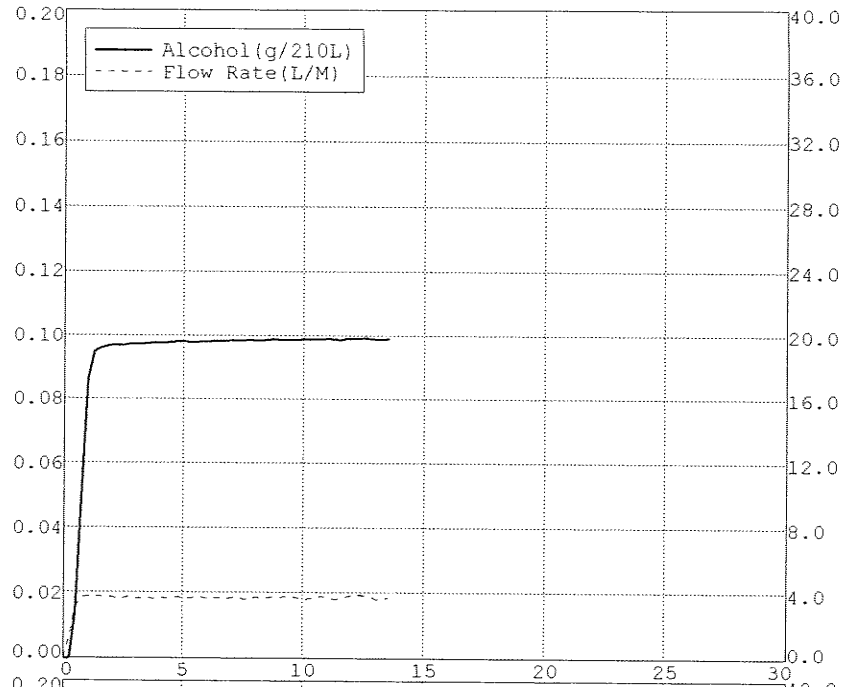

*Charles B. Geisler*  
#241