

SUPERVISOR TEST




WARREN COUNTY  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 144506

Date: 08/20/2019

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:00
INTERNAL STANDARD	VERIFIED	15:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:01
BLANK TEST	0.00	15:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:02
BLANK TEST	0.00	15:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:03
BLANK TEST	0.00	15:04

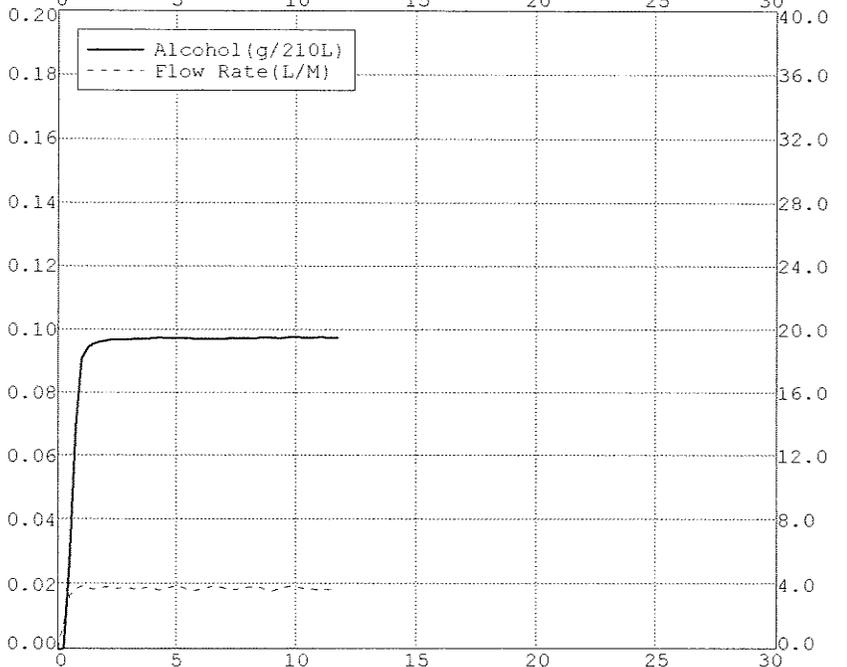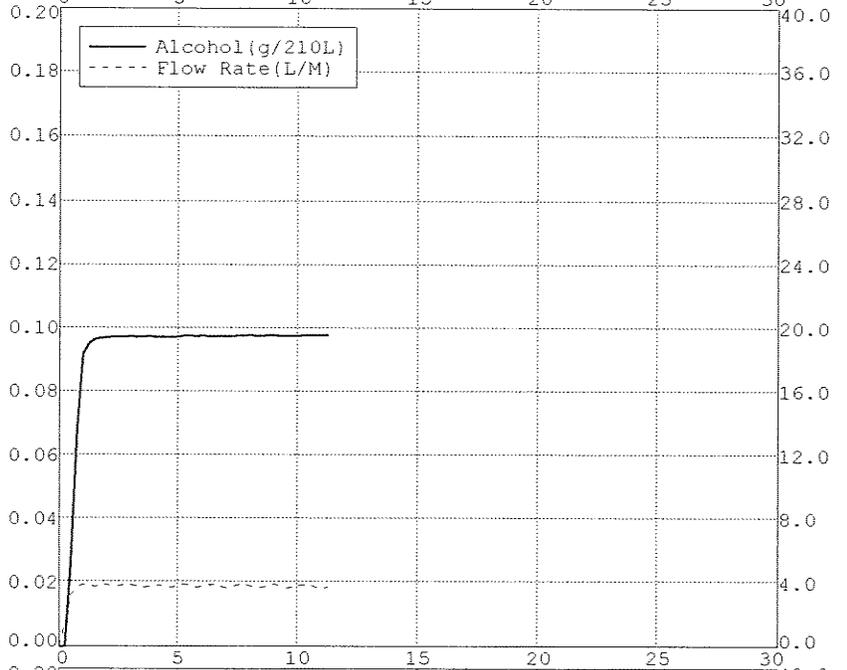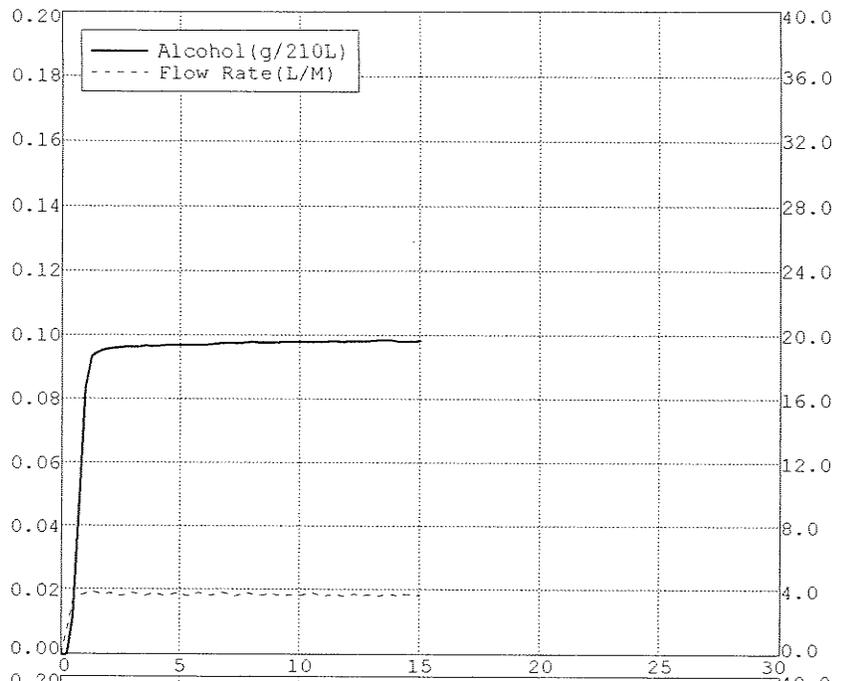

*Ch. B. Geisler* #201