

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 08/27/2019

OPERATOR NAME:
J T COON
Permit #: 36043
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:54
INTERNAL STANDARD	VERIFIED	04:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:55
BLANK TEST	0.00	04:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:56
BLANK TEST	0.00	04:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:57
BLANK TEST	0.00	04:58

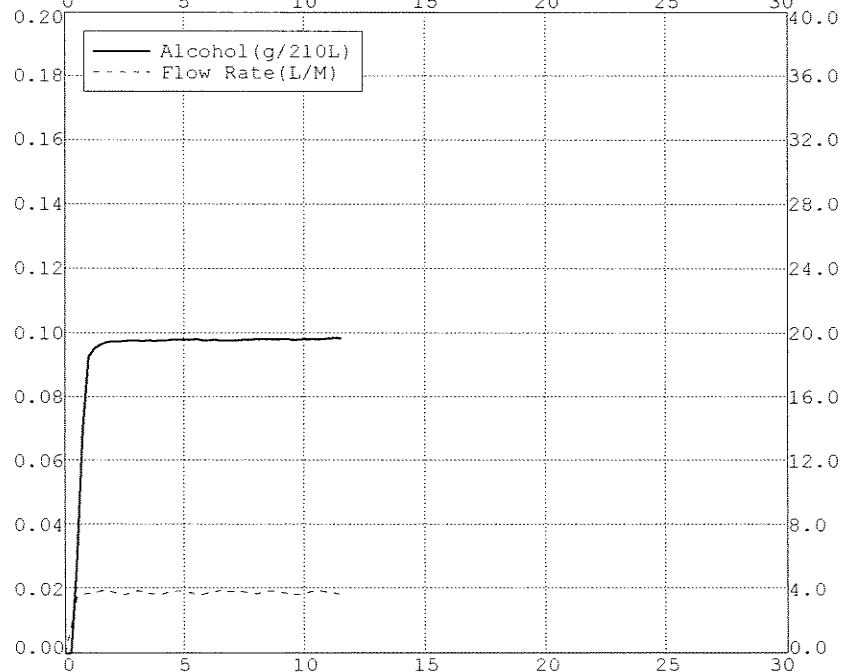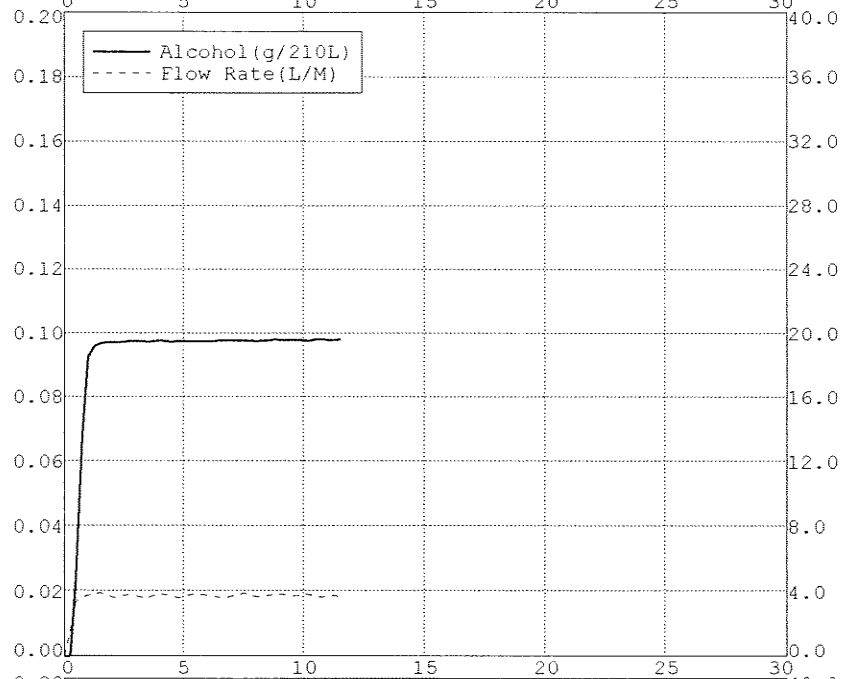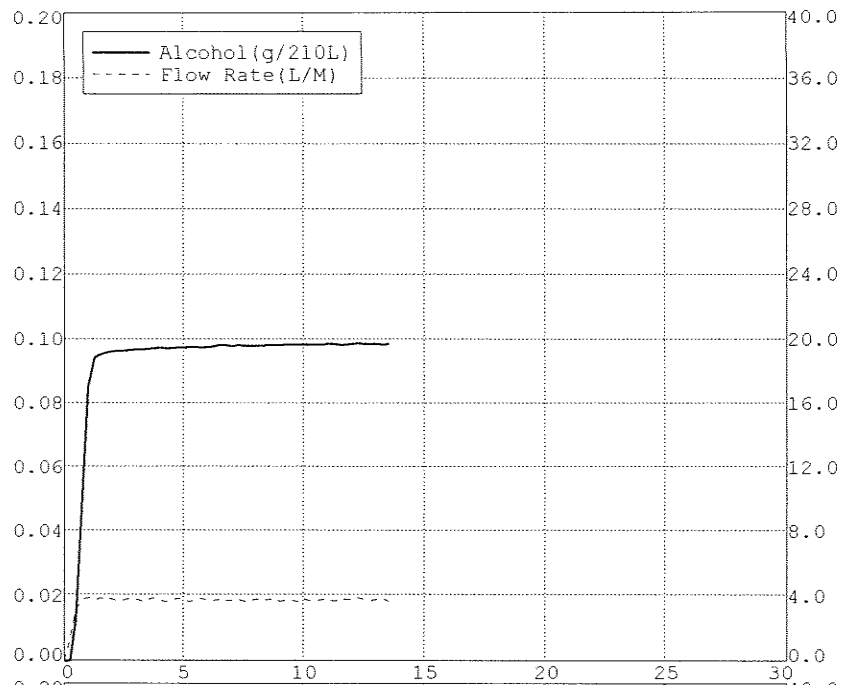

P.O. [Signature] 341