

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 09/09/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN COUNTY  
SHERIFF'S OFFICE  
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:36
INTERNAL STANDARD	VERIFIED	05:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:36
BLANK TEST	0.00	05:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:37
BLANK TEST	0.00	05:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:38
BLANK TEST	0.00	05:39

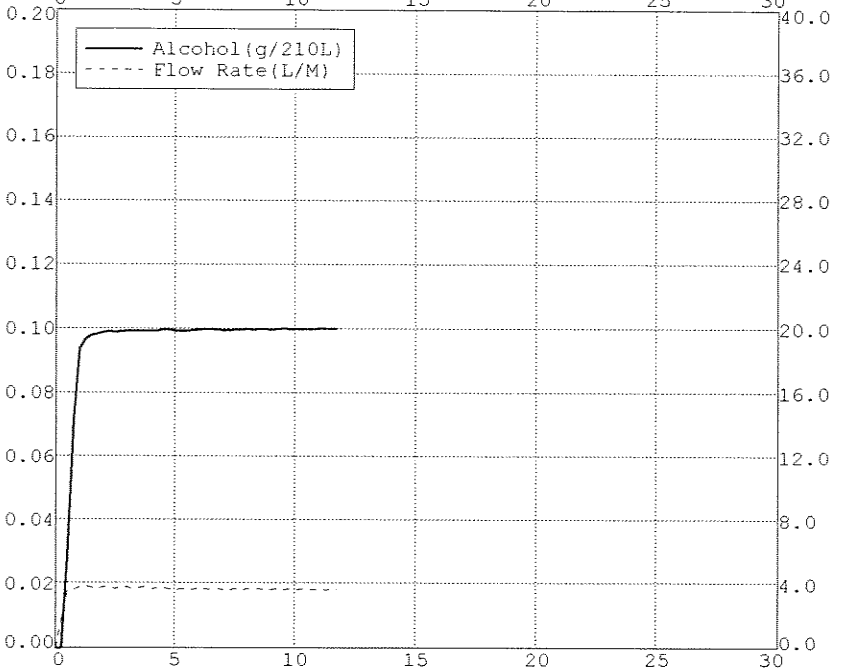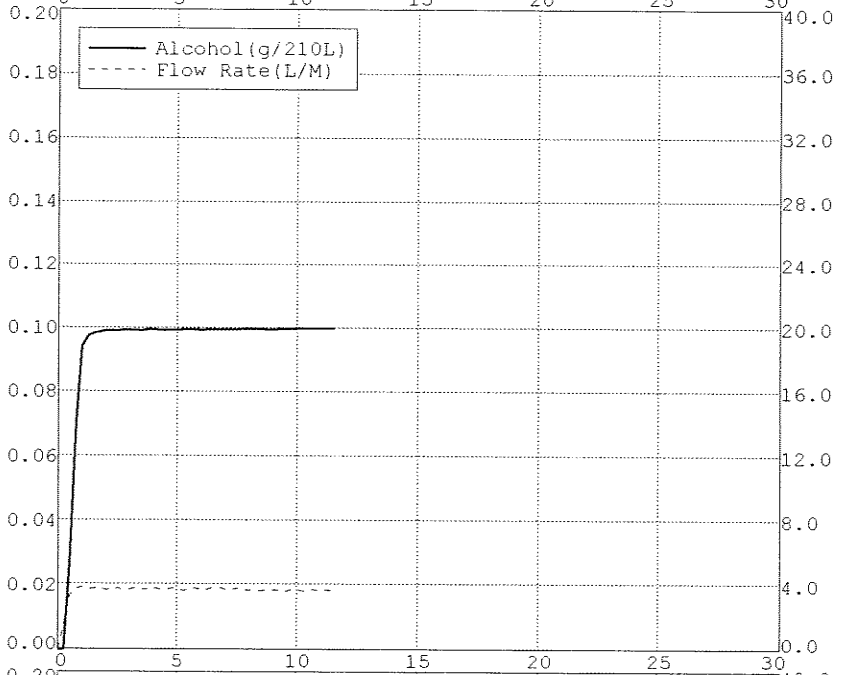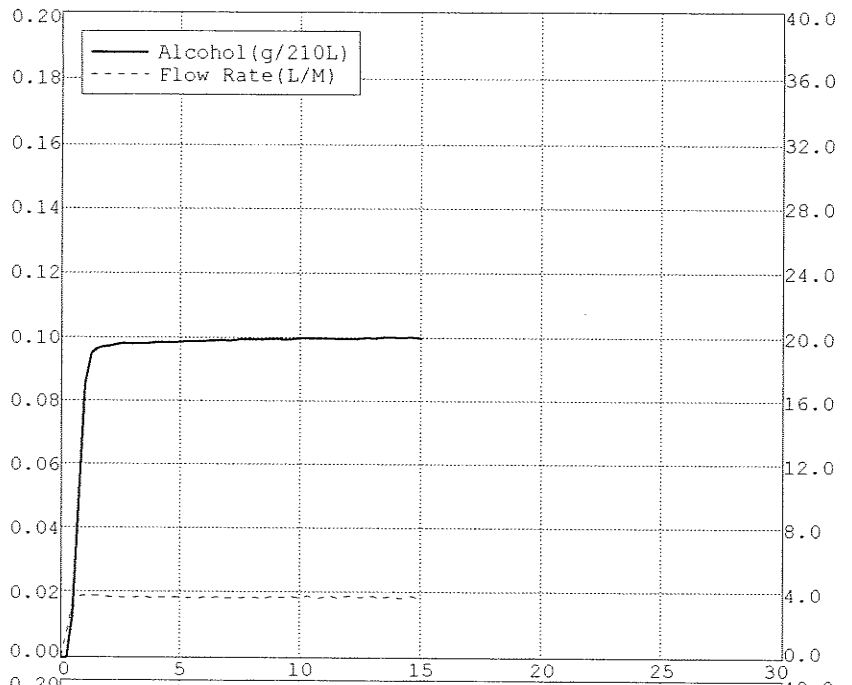

*Signature: Sgt. Charles B. Geisler #201*