

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 09/21/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:52
INTERNAL STANDARD	VERIFIED	05:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	05:52
BLANK TEST	0.00	05:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:53
BLANK TEST	0.00	05:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:54
BLANK TEST	0.00	05:55

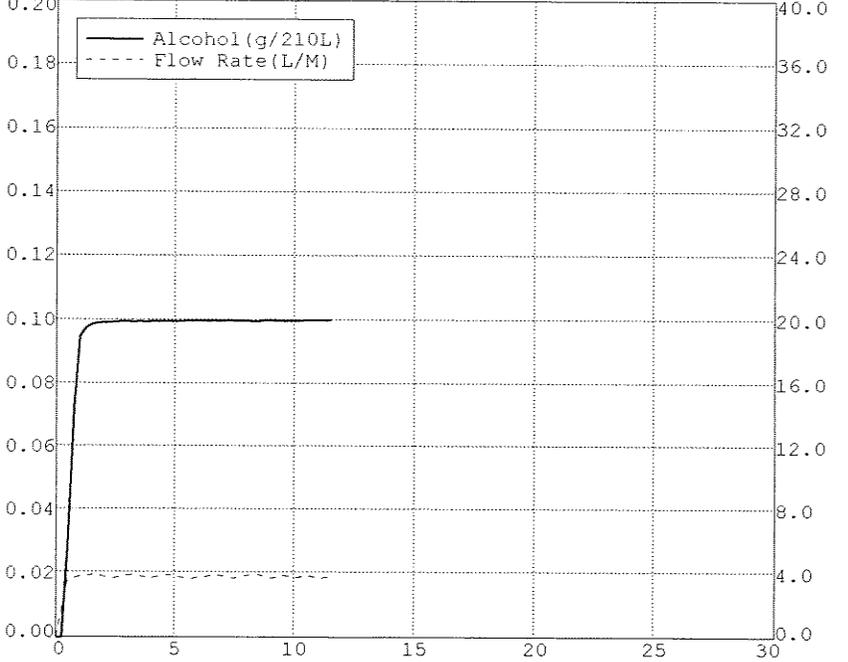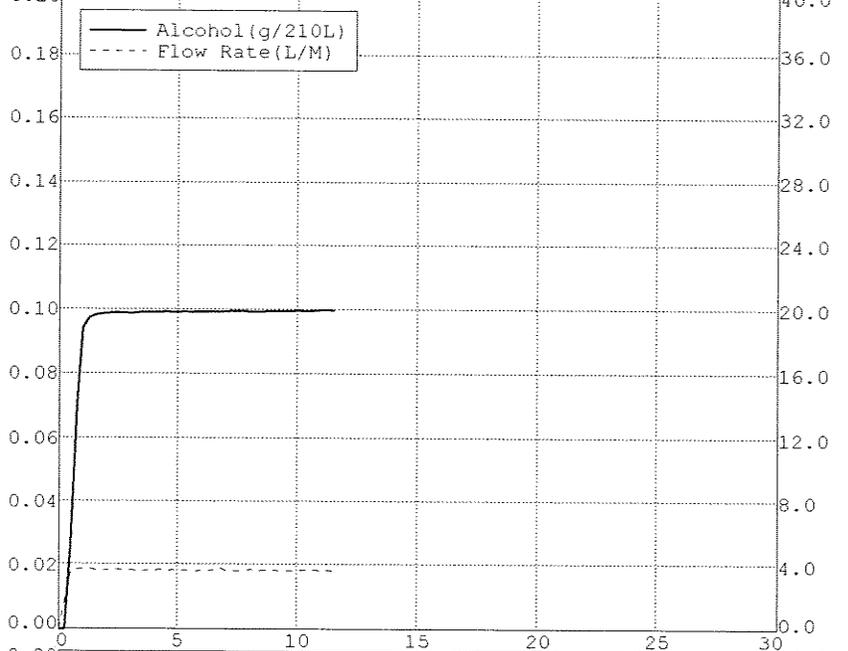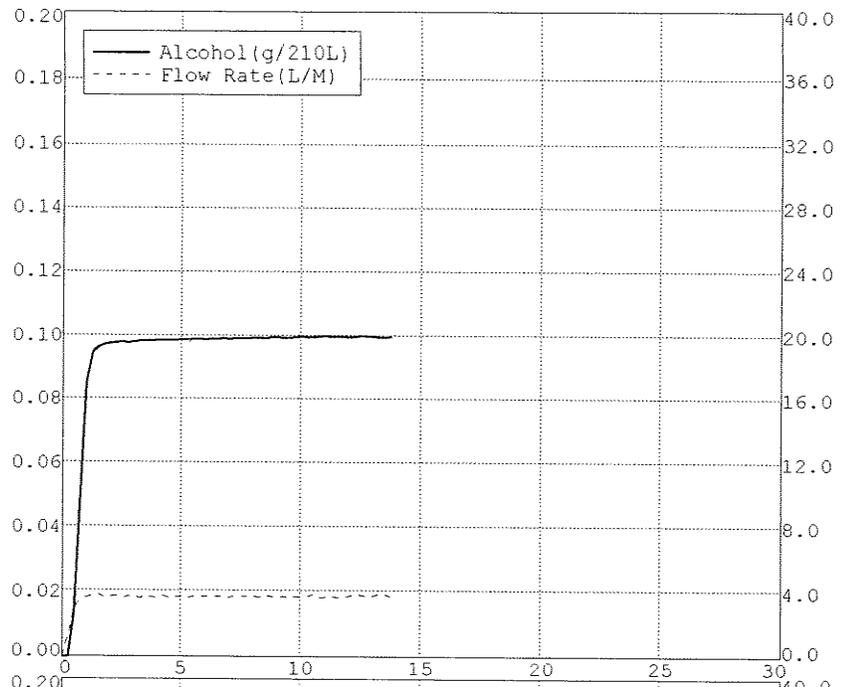

Handwritten signatures and initials:
C.B. Geisler
[Signature]