

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 10/09/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:45
INTERNAL STANDARD	VERIFIED	12:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:45
BLANK TEST	0.00	12:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:47
BLANK TEST	0.00	12:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:48
BLANK TEST	0.00	12:49

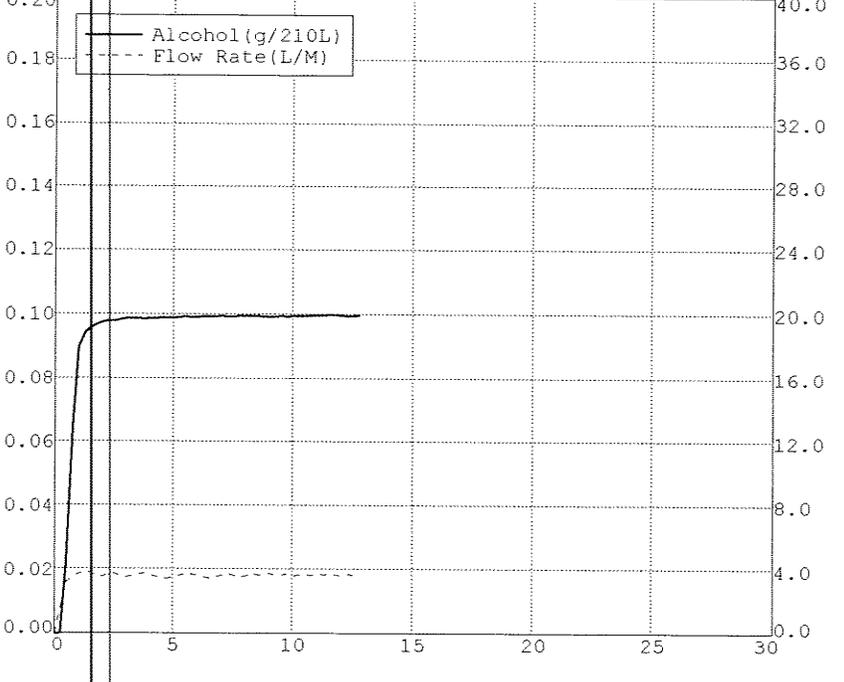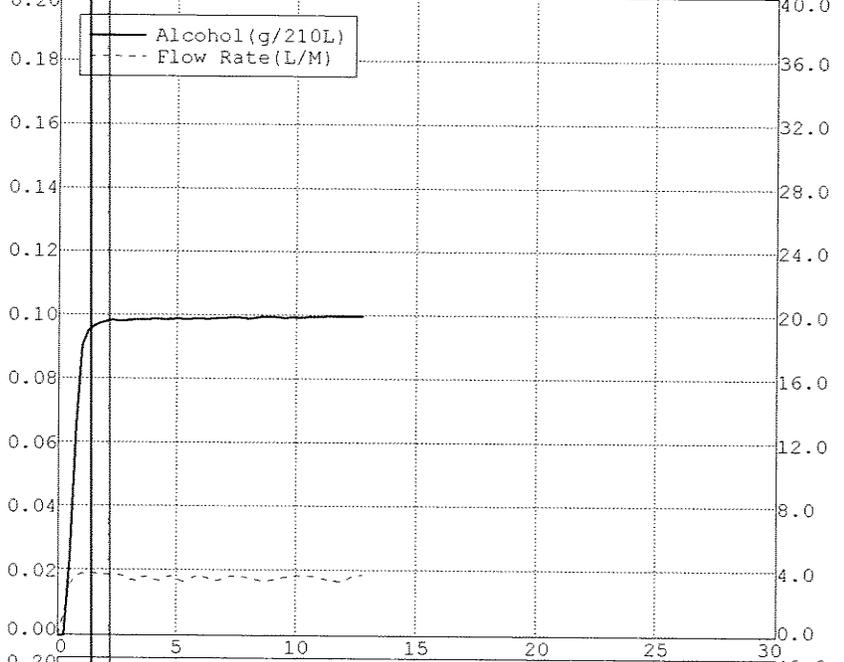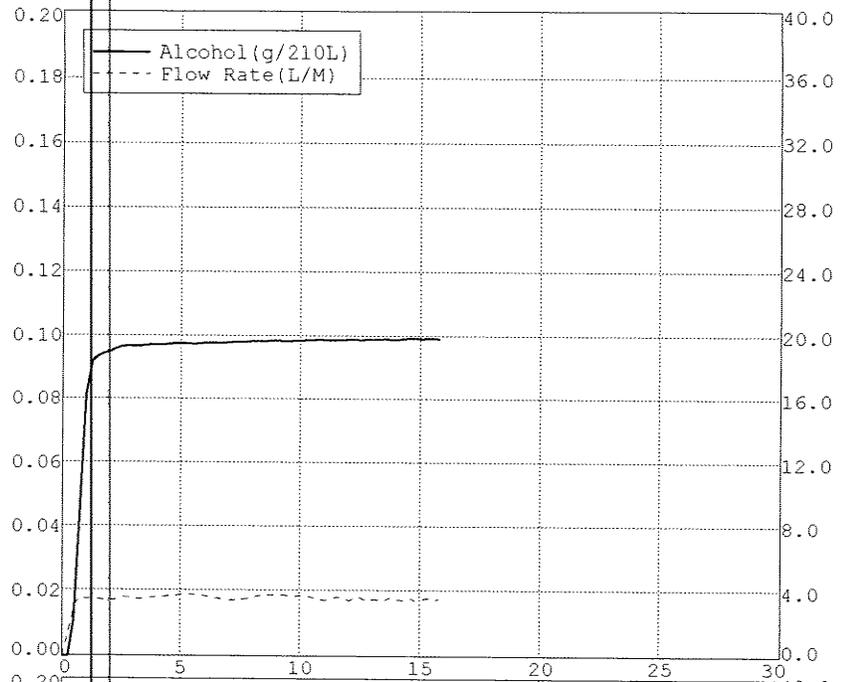

Handwritten signatures and initials:
A. [Signature] [Signature] [Signature]