

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 10/30/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:28
INTERNAL STANDARD	VERIFIED	03:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:29
BLANK TEST	0.00	03:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:30
BLANK TEST	0.00	03:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:31
BLANK TEST	0.00	03:32

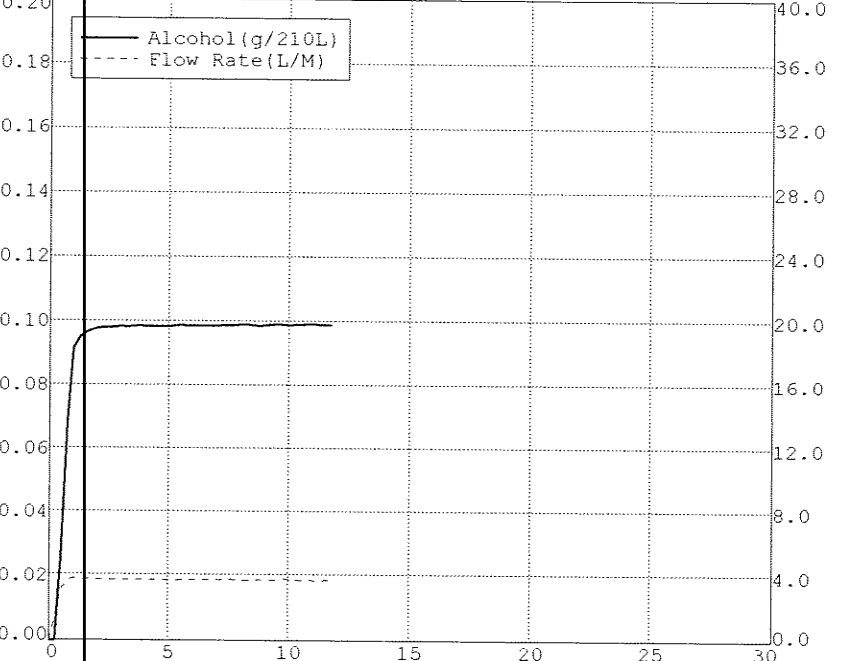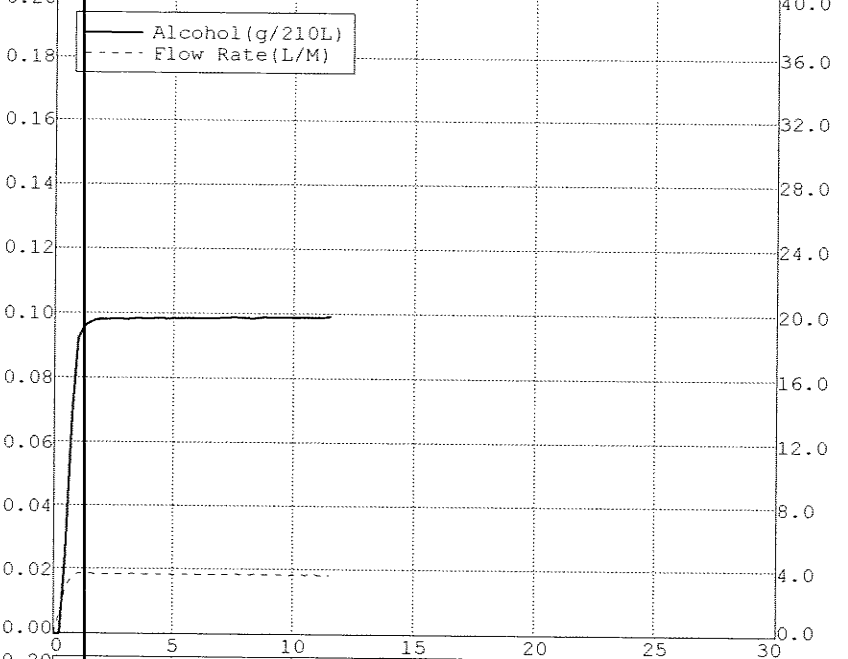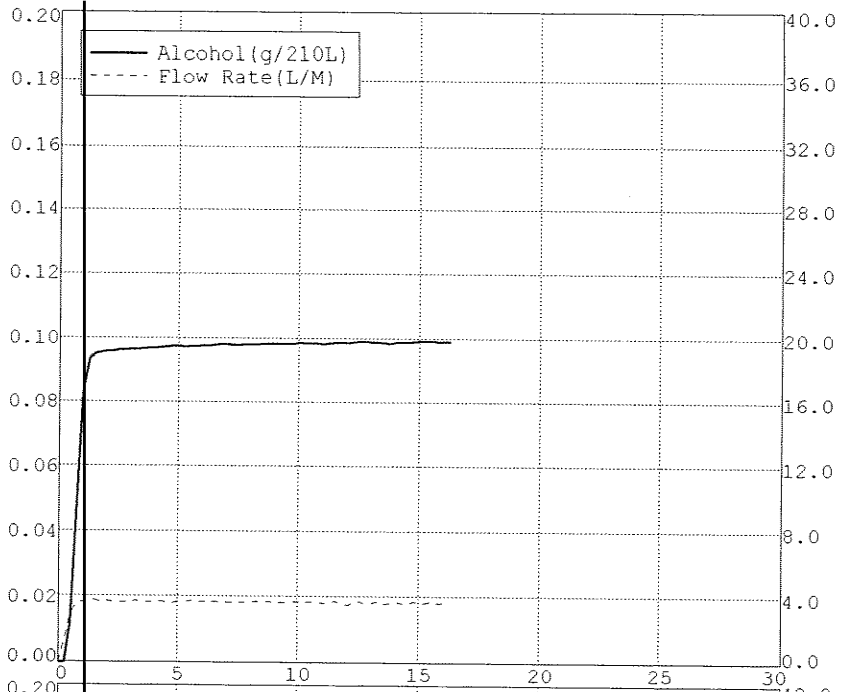

*Handwritten signature and initials: C. B. Geisler #24V*