

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 11/07/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:25
INTERNAL STANDARD	VERIFIED	12:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:25
BLANK TEST	0.00	12:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:26
BLANK TEST	0.00	12:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:27
BLANK TEST	0.00	12:28

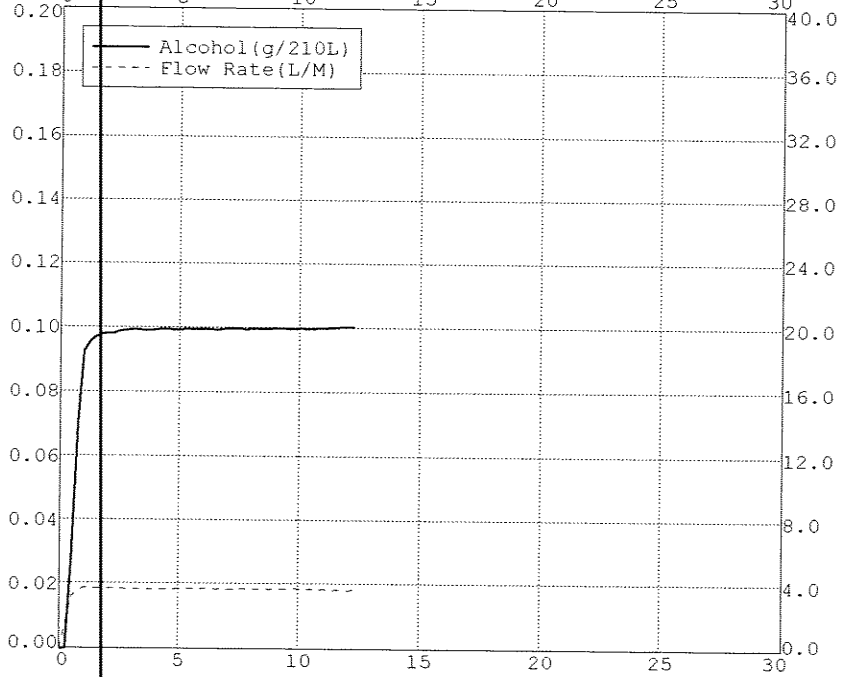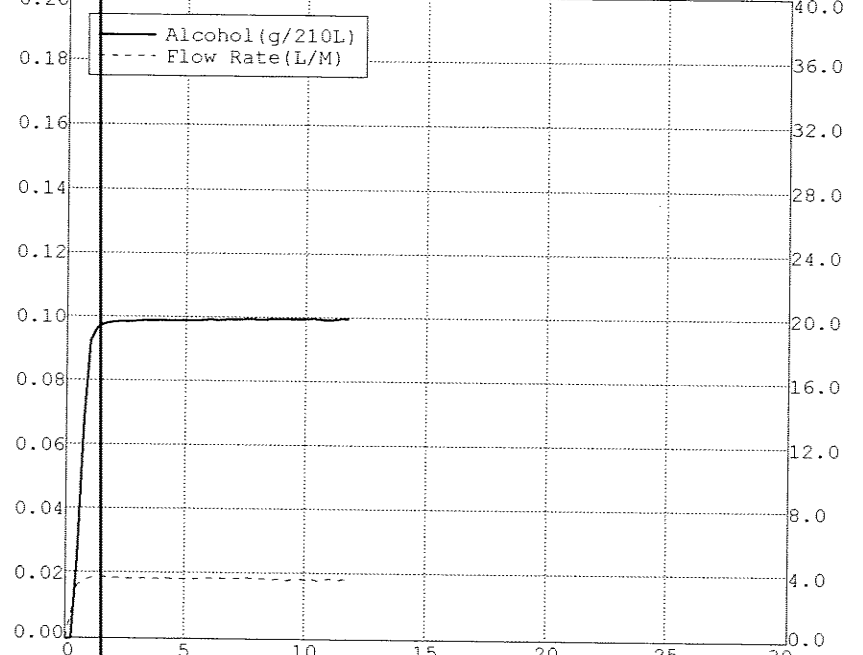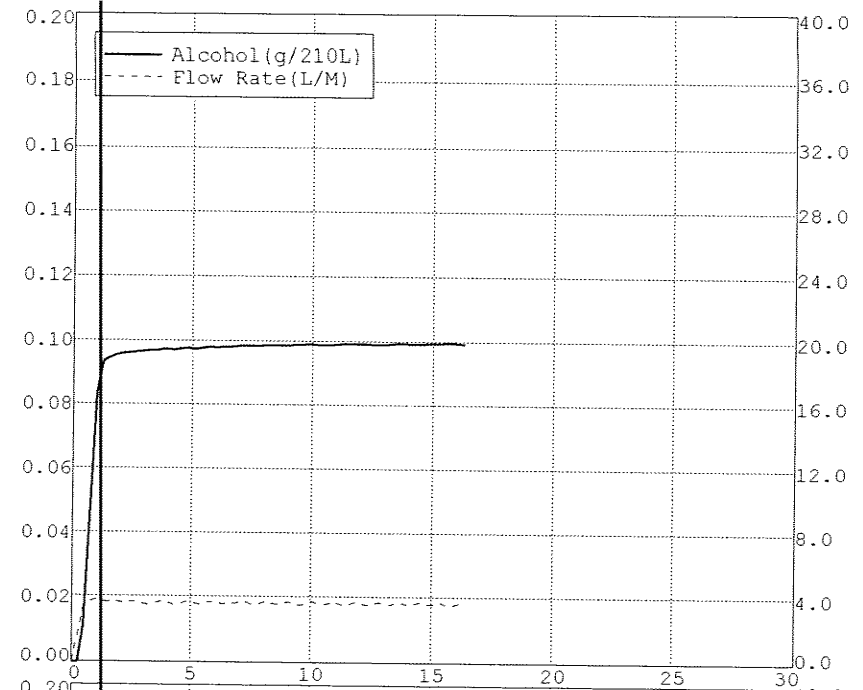

*Sgt. M. O. [Signature]* #22