

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 12/14/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:14
INTERNAL STANDARD	VERIFIED	06:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:15
BLANK TEST	0.00	06:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:16
BLANK TEST	0.00	06:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:17
BLANK TEST	0.00	06:18

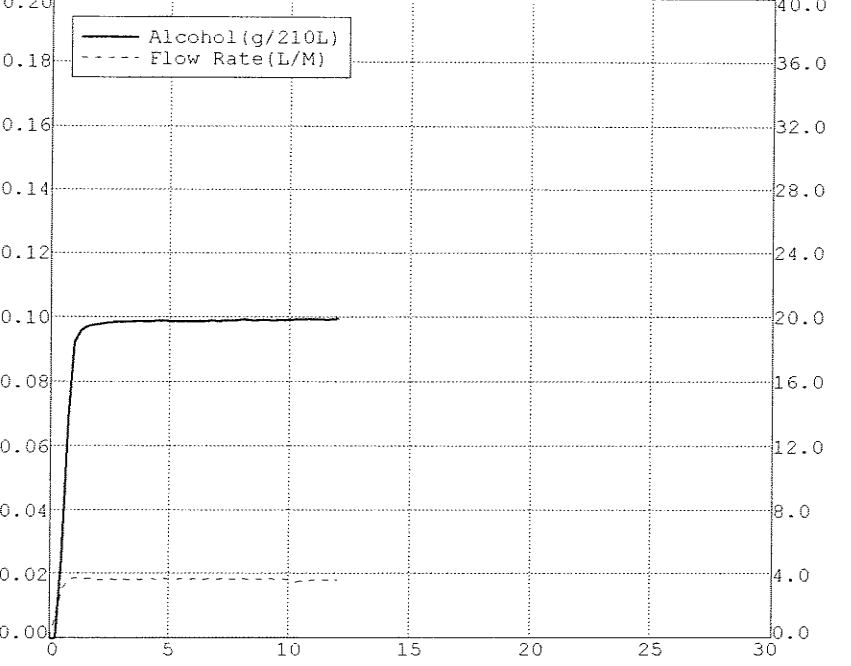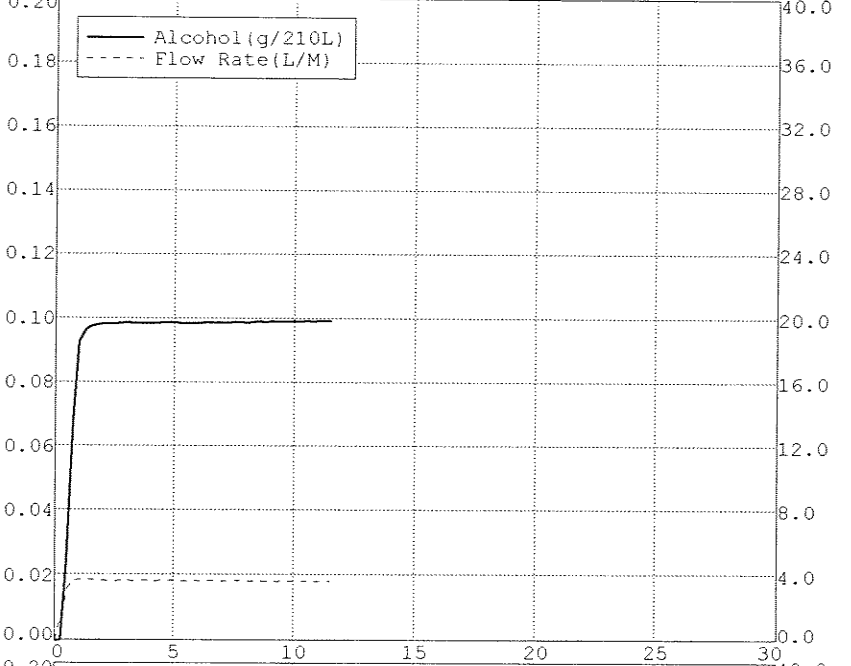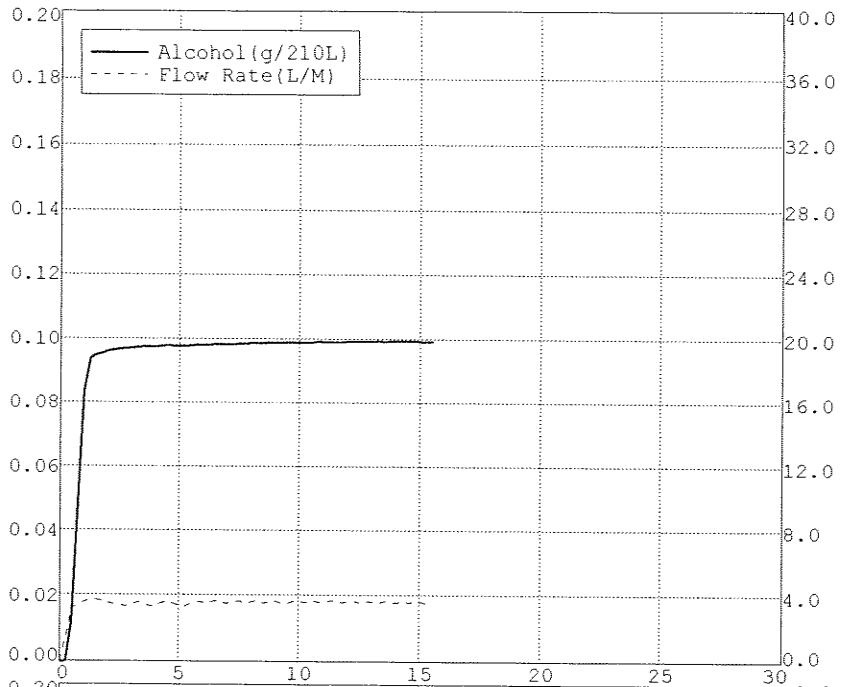

*Sgt. Charles B. Geisler #244*