

SOLUTION CHANGE




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 01/01/2020

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:34
INTERNAL STANDARD	VERIFIED	17:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:34
BLANK TEST	0.00	17:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:35
BLANK TEST	0.00	17:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:36
BLANK TEST	0.00	17:37

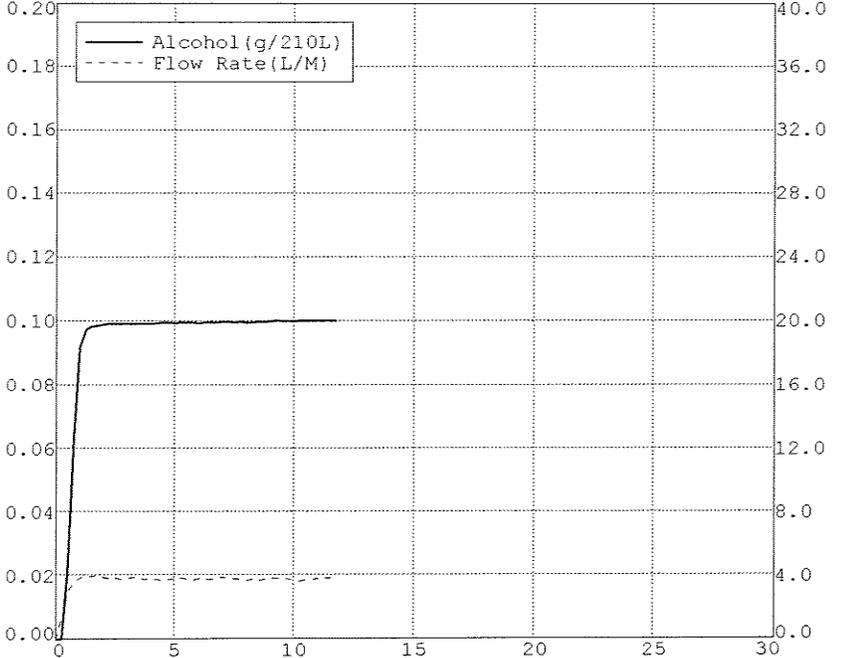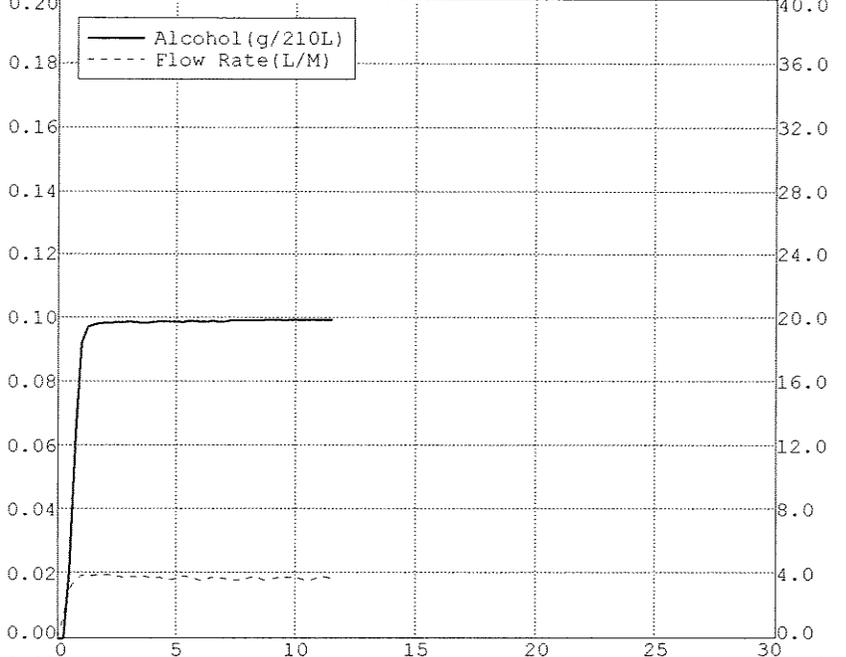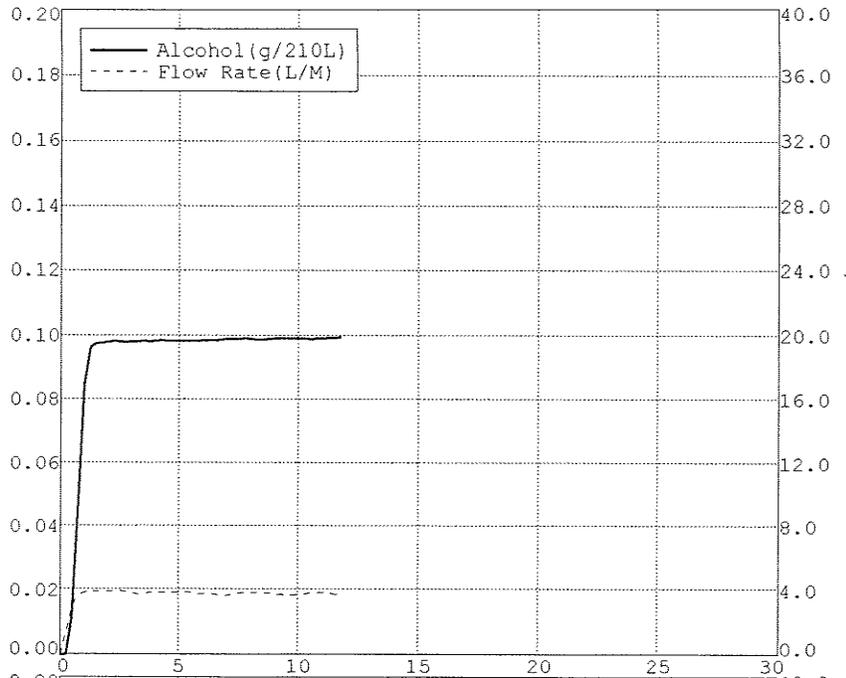

Charles B. Geisler