

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 01/06/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:29
INTERNAL STANDARD	VERIFIED	23:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:30
BLANK TEST	0.00	23:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:31
BLANK TEST	0.00	23:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:32
BLANK TEST	0.00	23:33

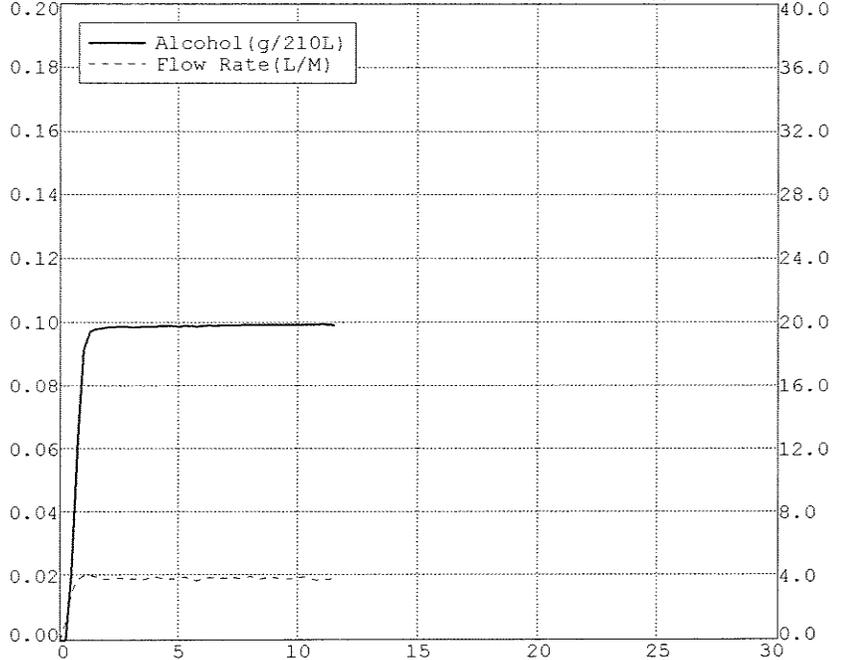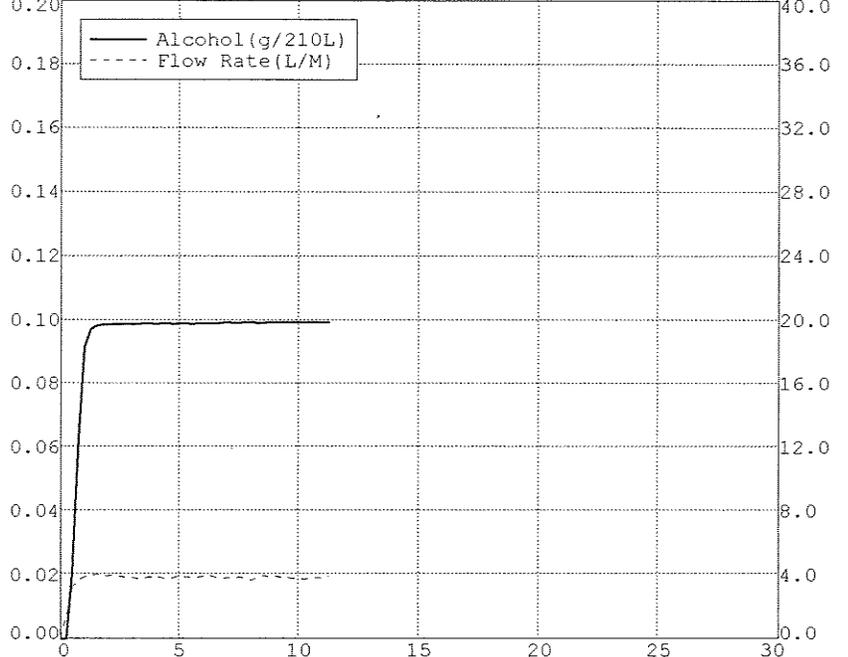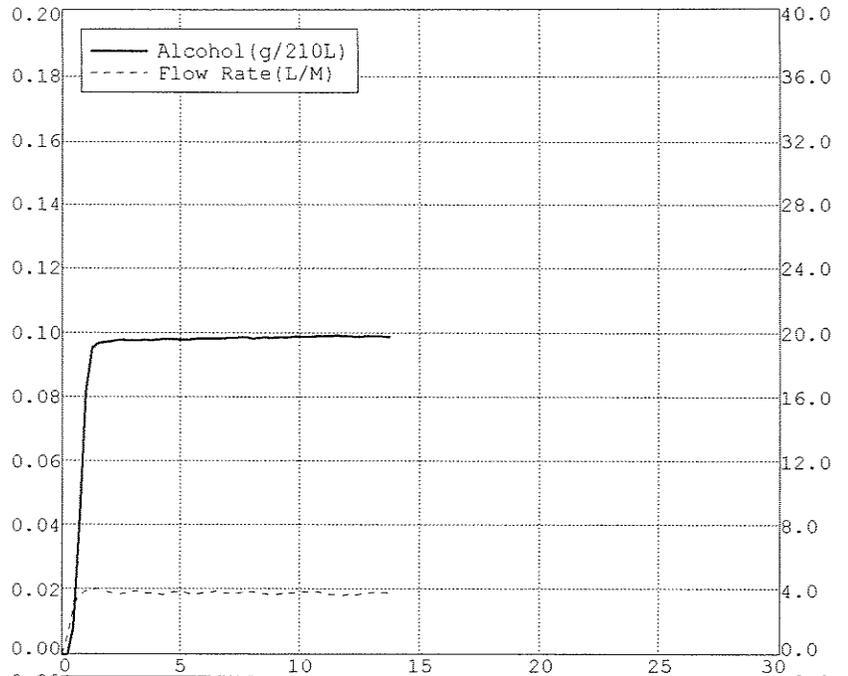

*Handwritten signature: Charles B. Geisler*